




## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification <sup>7</sup> : A61B 5/00	A1	(11) International Publication Number: WO 00/42911 (43) International Publication Date: 27 July 2000 (27.07.00)
(21) International Application Number: PCT/US00/01884 (22) International Filing Date: 25 January 2000 (25.01.00) (30) Priority Data: 60/117,097 25 January 1999 (25.01.99) US 60/161,565 26 October 1999 (26.10.99) US (71) Applicant: MASIMO CORPORATION [US/US]; 2852 Kelvin Avenue, Irvine, CA 92614 (US). (72) Inventors: KIANI, Massi, E.; 35 Brindisi, Laguna Niguel, CA 92677 (US). ALI, Ammar, Al; 10880 Phillips Street, Tustin, CA 92782 (US). DIAB, Mohamed, K.; 26945 Diamond, Mission Viejo, CA 92692 (US). VADEN, Val, E.; 70 Downey Way, Hillsborough, CA 94010 (US). (74) Agent: NATAUPSKY, Steven, J.; Knobbe, Martens, Olson and Bear, LLP, 620 Newport Center Drive, 16th Floor, Newport Beach, CA 92660 (US).		(81) Designated States: AU, BR, CA, DE, GB, JP, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).  <b>Published</b> <i>With international search report. Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i>

(54) Title: UNIVERSAL/UPGRADING PULSE OXIMETER

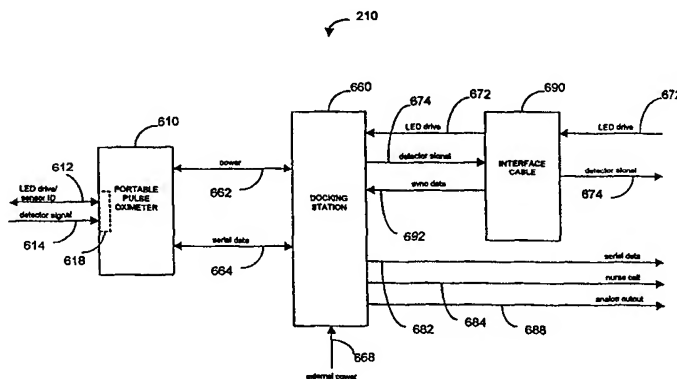

## (57) Abstract

A universal/upgrading pulse oximeter (UPO) (210) comprises a portable unit (610) and a docking station (660, 910) together providing three-instruments-in-one functionality for measuring oxygen saturation and related physiological parameters. The portable unit functions as a handheld pulse oximeter. The combination of the docked portable and the docking station functions as a stand-alone, high-performance pulse oximeter. The portable-docking station combination is also connectable to, and universally compatible with, pulse oximeters from various manufacturers through use of a waveform generator (320, 930). The UPO provides a universal sensor to pulse oximeter interface and a pulse oximeter measurement capability that upgrades the performance of conventional instruments by increasing low perfusion performance and motion artifact immunity, for example. Universal compatibility combined with portability allows the UPO to be transported along with patients transferred between an ambulance and a hospital ER, or between various hospital sites, providing continuous patient monitoring in addition to plug-compatibility and functional upgrading for multiparameter patient monitoring systems. The image on the portable display (264, 740) is rotatable, either manually when undocked or as a function of orientation (950). In one embodiment, the docking station (660) has a web server and network interface (1410) that allows UPO data to be downloaded and viewed as web pages over a local area network (1420) or the Internet.

***FOR THE PURPOSES OF INFORMATION ONLY***

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

## UNIVERSAL/UPGRADING PULSE OXIMETER

### Background of the Invention

Oximetry is the measurement of the oxygen level status of blood. Early detection of low blood oxygen level is critical in the medical field, for example in critical care and surgical applications, because an insufficient supply of oxygen can result in brain damage and death in a matter of minutes. Pulse oximetry is a widely accepted noninvasive procedure for measuring the oxygen saturation level of arterial blood, an indicator of oxygen supply. A pulse oximetry system consists of a sensor applied to a patient, a pulse oximeter, and a patient cable connecting the sensor and the pulse oximeter.

The pulse oximeter may be a standalone device or may be incorporated as a module or built-in portion of a multiparameter patient monitoring system, which also provides measurements such as blood pressure, respiratory rate and EKG. A pulse oximeter typically provides a numerical readout of the patient's oxygen saturation, a numerical readout of pulse rate, and an audible indicator or "beep" that occurs in response to each pulse. In addition, the pulse oximeter may display the patient's plethysmograph, which provides a visual display of the patient's pulse contour and pulse rate.

### Summary of the Invention

FIG. 1 illustrates a prior art pulse oximeter **100** and associated sensor **110**. Conventionally, a pulse oximetry sensor **110** has LED emitters **112**, typically one at a red wavelength and one at an infrared wavelength, and a photodiode detector **114**. The sensor **110** is typically attached to an adult patient's finger or an infant patient's foot. For a finger, the sensor **110** is configured so that the emitters **112** project light through the fingernail and through the blood vessels and capillaries underneath. The LED emitters **112** are activated by drive signals **122** from the pulse oximeter **100**. The detector **114** is positioned at the fingertip opposite the fingernail so as to detect the LED emitted light as it emerges from the finger tissues. The photodiode generated signal **124** is relayed by a cable to the pulse oximeter **100**.

The pulse oximeter **100** determines oxygen saturation ( $\text{SpO}_2$ ) by computing the differential absorption by arterial blood of the two wavelengths emitted by the sensor **110**. The pulse oximeter **100** contains a sensor interface **120**, an  $\text{SpO}_2$  processor **130**, an instrument manager **140**, a display **150**, an audible indicator (tone generator) **160** and a keypad **170**. The sensor interface **120** provides LED drive current **122** which alternately activates the sensor red and IR LED emitters **112**. The sensor interface **120** also has input circuitry for amplification and filtering of the signal **124** generated by the photodiode detector **114**, which corresponds to the red and infrared light energy attenuated from transmission through the patient tissue site. The  $\text{SpO}_2$  processor **130** calculates a ratio of detected red and infrared intensities, and an arterial oxygen saturation value is empirically determined based on that ratio. The instrument manager **140** provides hardware and software interfaces for managing the display **150**, audible indicator **160** and keypad **170**. The display **150** shows the computed oxygen status, as described above. The audible indicator **160** provides the pulse beep as well as alarms indicating desaturation events. The keypad **170** provides a user interface for such things as alarm thresholds, alarm enablement, and display options.

Computation of  $\text{SpO}_2$  relies on the differential light absorption of oxygenated hemoglobin,  $\text{HbO}_2$ , and deoxygenated hemoglobin, Hb, to determine their respective concentrations in the arterial blood. Specifically, pulse

oximetry measurements are made at red and IR wavelengths chosen such that deoxygenated hemoglobin absorbs more red light than oxygenated hemoglobin, and, conversely, oxygenated hemoglobin absorbs more infrared light than deoxygenated hemoglobin, for example 660 nm (red) and 905 nm (IR).

To distinguish between tissue absorption at the two wavelengths, the red and IR emitters 112 are provided drive current 122 so that only one is emitting light at a given time. For example, the emitters 112 may be cycled on and off alternately, in sequence, with each only active for a quarter cycle and with a quarter cycle separating the active times. This allows for separation of red and infrared signals and removal of ambient light levels by downstream signal processing. Because only a single detector 114 is used, it responds to both the red and infrared emitted light and generates a time-division-multiplexed ("modulated") output signal 124. This modulated signal 124 is coupled to the input of the sensor interface 120.

In addition to the differential absorption of hemoglobin derivatives, pulse oximetry relies on the pulsatile nature of arterial blood to differentiate hemoglobin absorption from absorption of other constituents in the surrounding tissues. Light absorption between systole and diastole varies due to the blood volume change from the inflow and outflow of arterial blood at a peripheral tissue site. This tissue site might also comprise skin, muscle, bone, venous blood, fat, pigment, etc., each of which absorbs light. It is assumed that the background absorption due to these surrounding tissues is invariant and can be ignored. Thus, blood oxygen saturation measurements are based upon a ratio of the time-varying or AC portion of the detected red and infrared signals with respect to the time-invariant or DC portion:

$$RD/IR = (Red_{AC}/Red_{DC})/(IR_{AC}/IR_{DC})$$

The desired SpO<sub>2</sub> measurement is then computed from this ratio. The relationship between RD/IR and SpO<sub>2</sub> is most accurately determined by statistical regression of experimental measurements obtained from human volunteers and calibrated measurements of oxygen saturation. In a pulse oximeter device, this empirical relationship can be stored as a "calibration curve" in a read-only memory (ROM) look-up table so that SpO<sub>2</sub> can be directly read-out of the memory in response to input RD/IR measurements.

Pulse oximetry is the standard-of-care in various hospital and emergency treatment environments. Demand has lead to pulse oximeters and sensors produced by a variety of manufacturers. Unfortunately, there is no standard for either performance by, or compatibility between, pulse oximeters or sensors. As a result, sensors made by one manufacturer are unlikely to work with pulse oximeters made by another manufacturer. Further, while conventional pulse oximeters and sensors are incapable of taking measurements on patients with poor peripheral circulation and are partially or fully disabled by motion artifact, advanced pulse oximeters and sensors manufactured by the assignee of the present invention are functional under these conditions. This presents a dilemma to hospitals and other caregivers wishing to upgrade their patient oxygenation monitoring capabilities. They are faced with either replacing all of their conventional pulse oximeters, including multiparameter patient monitoring systems, or working with potentially incompatible sensors and inferior pulse oximeters manufactured by various vendors for the pulse oximetry equipment in use at the installation.

Hospitals and other caregivers are also plagued by the difficulty of monitoring patients as they are transported from one setting to another. For example, a patient transported by ambulance to a hospital emergency room will likely be

unmonitored during the transition from ambulance to the ER and require the removal and replacement of incompatible sensors in the ER. A similar problem is faced within a hospital as a patient is moved between surgery, ICU and recovery settings. Incompatibility and transport problems are exacerbated by the prevalence of expensive and non-portable multiparameter patient monitoring systems having pulse oximetry modules as one measurement parameter.

5           The Universal/Upgrading Pulse Oximeter (UPO) according to the present invention is focused on solving these performance, incompatibility and transport problems. The UPO provides a transportable pulse oximeter that can stay with and continuously monitor the patient as they are transported from setting to setting. Further, the UPO provides a synthesized output that drives the sensor input of other pulse oximeters. This allows the UPO to function as a universal interface that matches incompatible sensors with other pulse oximeter instruments. Further, the UPO acts as an upgrade  
10           to existing pulse oximeters that are adversely affected by low tissue perfusion and motion artifact. Likewise, the UPO can drive a SpO<sub>2</sub> sensor input of multiparameter patient monitoring systems, allowing the UPO to integrate into the associated multiparameter displays, patient record keeping systems and alarm management functions.

          One aspect of the present invention is a measurement apparatus comprising a sensor, a first pulse oximeter and a waveform generator. The sensor has at least one emitter and an associated detector configured to attach to a  
15           tissue site. The detector provides an intensity signal responsive to the oxygen content of arterial blood at the tissue site. The first pulse oximeter is in communication with the detector and computes an oxygen saturation measurement based on the intensity signal. The waveform generator is in communication with the first pulse oximeter and provides a waveform based on the oxygen saturation measurement. A second pulse oximeter is in communication with the waveform generator and displays an oxygen saturation value based on the waveform. The waveform is synthesized so  
20           that the oxygen saturation value is generally equivalent to the oxygen saturation measurement.

          In another aspect of the present invention, a measurement apparatus comprises a first sensor port connectable to a sensor, an upgrade port, a signal processor and a waveform generator. The upgrade port is connectable to a second sensor port of a physiological monitoring apparatus. The signal processor is configured to compute a physiological measurement based on a signal input to the first sensor port. The waveform generator  
25           produces a waveform based on the physiological measurement, and the waveform is available at the upgrade port. The waveform is adjustable so that the physiological monitoring apparatus displays a value generally equivalent to the physiological measurement when the upgrade port is attached to the second sensor port.

          Yet another aspect of the present invention is a measurement method comprising the steps of sensing an intensity signal responsive to the oxygen content of arterial blood at a tissue site and computing an oxygen saturation  
30           measurement based on the intensity signal. Other steps are generating a waveform based on the oxygen saturation measurement and providing the waveform to the sensor inputs of a pulse oximeter so that the pulse oximeter displays an oxygen saturation value generally equivalent to the oxygen saturation measurement.

          An additional aspect of the present invention is a measurement method comprising the steps of sensing a  
35           physiological signal, computing a physiological measurement based upon the signal, and synthesizing a waveform as a function of the physiological measurement. A further step is outputting the waveform to a sensor input of a

physiological monitoring apparatus. The synthesizing step is performed so that the measurement apparatus displays a value corresponding to the physiological measurement.

A further aspect of the present invention is a measurement apparatus comprising a first pulse oximeter for making an oxygen saturation measurement and a pulse rate measurement based upon an intensity signal derived from a tissue site. Also included is a waveform generation means for creating a signal based upon the oxygen saturation measurement and the pulse rate measurement. In addition, there is a communication means for transmitting the signal to a second pulse oximeter.

Another aspect of the present invention is a measurement apparatus comprising a portable portion having a sensor port, a processor, a display, and a docking connector. The sensor port is configured to receive an intensity signal responsive to the oxygen content of arterial blood at a tissue site. The processor is programmed to compute an oxygen saturation value based upon the intensity signal and to output the value to the display. A docking station has a portable connector and is configured to accommodate the portable so that the docking connector mates with the portable connector. This provides electrical connectivity between the docking station and the portable. The portable has an undocked position separate from the docking station in which the portable functions as a handheld pulse oximeter. The portable also has a docked position at least partially retained within the docking station in which the combination of the portable and the docking station has at least one additional function compared with the portable in the undocked position.

A further aspect of the present invention is a measurement apparatus configured to function in both a first spatial orientation and a second spatial orientation. The apparatus comprises a sensor port configured to receive a signal responsive to a physiological state. The apparatus also has a tilt sensor providing an output responsive to gravity. In addition, there is a processor in communication with the sensor port and the tilt sensor output. The processor is programmed to compute a physiological measurement value based upon the signal and to determine whether the measurement apparatus is in the first orientation or the second orientation based upon the tilt sensor output. A display has a first mode and a second mode and is driven by the processor. The display shows the measurement value in the first mode when the apparatus is in the first orientation and shows the measurement value in the second mode when the apparatus is in the second orientation.

Another aspect of the present invention is a measurement method comprising the steps of sensing a signal responsive to a physiological state and computing physiological measurement based on the signal. Additional steps are determining the spatial orientation of a tilt sensor and displaying the physiological measurement in a mode that is based upon the determining step.

#### Brief Description of the Drawings

FIG. 1 is a block diagram of a prior art pulse oximeter;

FIG. 2 is a diagram illustrating a patient monitoring system incorporating a universal/upgrading pulse oximeter (UPO) according to the present invention;

FIG. 3 is top level block diagram of a UPO embodiment;

FIG. 4 is a detailed block diagram of the waveform generator portion of the UPO embodiment shown in FIG. 3;

FIG. 5 is an illustration of a handheld embodiment of the UPO;

FIG. 6 is a top level block diagram of another UPO embodiment incorporating a portable pulse oximeter and a docking station;

FIG. 7 is a detailed block diagram of the portable pulse oximeter portion of FIG. 6;

FIG. 8A is an illustration of the portable pulse oximeter user interface, including a keyboard and display;

FIGS. 8B-C are illustrations of the portable pulse oximeter display showing portrait and landscape modes, respectively;

FIG. 9 is a detailed block diagram of the docking station portion of FIG. 6;

FIG. 10 is a schematic of the interface cable portion of FIG. 6;

FIG. 11A is a front view of an embodiment of a portable pulse oximeter;

FIG. 11B is a back view of a portable pulse oximeter;

FIG. 12A is a front view of an embodiment of a docking station;

FIG. 12B is a back view of a docking station;

FIG. 13 is a front view of a portable docked to a docking station; and

FIG. 14 is a block diagram of one embodiment of a local area network interface for a docking station.

#### Detailed Description of the Preferred Embodiments

FIG. 2 depicts the use of a Universal/Upgrading Pulse Oximeter ("UPO") 210 to perform patient monitoring. A pulse oximetry sensor 110 is attached to a patient (not illustrated) and provides the UPO 210 with a modulated red and IR photo-plethysmograph signal through a patient cable 220. The UPO 210 computes the patient's oxygen saturation and pulse rate from the sensor signal and, optionally, displays the patient's oxygen status. The UPO 210 may incorporate an internal power source 212, such as common alkaline batteries or a rechargeable power source. The UPO 210 may also utilize an external power source 214, such as standard 110V AC coupled with an external step-down transformer and an internal or external AC-to-DC converter.

In addition to providing pulse oximetry measurements, the UPO 210 also separately generates a signal, which is received by a pulse oximeter 268 external to the UPO 210. This signal is synthesized from the saturation calculated by the UPO 210 such that the external pulse oximeter 268 calculates the equivalent saturation and pulse rate as computed by the UPO 210. The external pulse oximeter 268 receiving the UPO signal may be a multiparameter patient monitoring system (MPMS) 260 incorporating a pulse oximeter module 268, a standalone pulse oximeter instrument, or any other host instrument capable of measuring SpO<sub>2</sub>. The MPMS 260 depicted in FIG. 2 has a rack 262 containing a number of modules for monitoring such patient parameters as blood pressure, EKG, respiratory gas, and SpO<sub>2</sub>. The measurements made by these various modules are shown on a multiparameter display 264, which is typically a video (CRT) device. The UPO 210 is connected to an existing MPMS 260 with a cable 230, advantageously integrating the UPO oxygen status measurements with other MPMS measurements. This allows the UPO calculations to be shown on a unified display of important patient parameters, networked with other patient data,

archived within electronic patient records and incorporated into alarm management, which are all MPMS functions convenient to the caregiver.

FIG. 3 depicts the major functions of the UPO 210, including an internal pulse oximeter 310, a waveform generator 320, a power supply 330 and an optional display 340. Attached to the UPO 210 is a sensor 110 and an external pulse oximeter 260. The internal pulse oximeter 310 provides the sensor 110 with a drive signal 312 that alternately activates the sensor's red and IR LEDs, as is well-known in the art. A corresponding detector signal 314 is received by the internal pulse oximeter 310. The internal pulse oximeter 310 computes oxygen saturation, pulse rate, and, in some embodiments, other physiological parameters such as pulse occurrence, plethysmograph features and measurement confidence. These parameters 318 are output to the waveform generator 320. A portion of these parameters may also be used to generate display drive signals 316 so that patient status may be read from, for example, an LED or LCD display module 340 on the UPO.

The internal pulse oximeter 310 may be a conventional pulse oximeter or, for upgrading an external pulse oximeter 260, it may be an advanced pulse oximeter capable of low perfusion and motion artifact performance not found in conventional pulse oximeters. An advanced pulse oximeter for use as an internal pulse oximeter 310 is described in U.S. Patent No. 5,632,272 assigned to the assignee of the present invention and incorporated herein by reference. An advanced pulse oximetry sensor for use as the sensor 110 attached to the internal pulse oximeter 310 is described in U.S. Patent No. 5,638,818 assigned to the assignee of the present invention and incorporated herein by reference. Further, a line of advanced Masimo SET<sup>®</sup> pulse oximeter OEM boards and sensors are available from the assignee of the present invention.

The waveform generator 320 synthesizes a waveform, such as a triangular waveform having a sawtooth or symmetric triangle shape, that is output as a modulated signal 324 in response to an input drive signal 322. The drive input 322 and modulation output 324 of the waveform generator 320 are connected to the sensor port 262 of the external pulse oximeter 260. The synthesized waveform is generated in a manner such that the external pulse oximeter 260 computes and displays a saturation and a pulse rate value that is equivalent to that measured by the internal pulse oximeter 310 and sensor 110. In the present embodiment, the waveforms for pulse oximetry are chosen to indicate to the external pulse oximeter 260 a perfusion level of 5%. The external pulse oximeter 260, therefore, always receives a strong signal. In an alternative embodiment, the perfusion level of the waveforms synthesized for the external pulse oximeter can be set to indicate a perfusion level at or close to the perfusion level of the patient being monitored by the internal pulse oximeter 310. As an alternative to the generated waveform, a digital data output 326, is connected to the data port 264 of the external pulse oximeter 260. In this manner, saturation and pulse rate measurements and also samples of the unmodulated, synthesized waveform can be communicated directly to the external pulse oximeter 260 for display, bypassing the external pulse oximeter's signal processing functions. The measured plethysmograph waveform samples output from the internal pulse oximeter 310 also may be communicated through the digital data output 326 to the external pulse oximeter 260.



It will be understood from the above discussion that the synthesized waveform is not physiological data from the patient being monitored by the internal pulse oximeter 310, but is a waveform synthesized from predetermined stored waveform data to cause the external pulse oximeter 260 to calculate oxygen saturation and pulse rate equivalent to or generally equivalent (within clinical significance) to that calculated by the internal pulse oximeter 310.

5 The actual physiological waveform from the patient received by the detector is not provided to the external pulse oximeter 260 in the present embodiment. Indeed, the waveform provided to the external pulse oximeter will usually not resemble the plethysmographic waveform of physiological data from the patient being monitored by the internal pulse oximeter 260.

The cable 230 (FIG. 2) attached between the waveform generator 320 and external pulse oximeter 260 provides a monitor ID 328 to the UPO, allowing identification of predetermined external pulse oximeter calibration curves. For example, this cable may incorporate an encoding device, such as a resistor, or a memory device, such as a PROM 1010 (FIG. 10) that is read by the waveform generator 320. The encoding device provides a value that uniquely identifies a particular type of external pulse oximeter 260 having known calibration curve, LED drive and modulation signal characteristics. Although the calibration curves of the external pulse oximeter 260 are taken into account, the wavelengths of the actual sensor 110, advantageously, are not required to correspond to the particular calibration curve indicated by the monitor ID 328 or otherwise assumed for the external pulse oximeter 260. That is, the wavelength of the sensor 110 attached to the internal pulse oximeter 310 is not relevant or known to the external pulse oximeter 260.

FIG. 4 illustrates one embodiment of the waveform generator portion 320 of the UPO 210 (FIG. 3). Although this embodiment is illustrated and described as hardware, one of ordinary skill will recognize that the functions of the waveform generator may be implemented in software or firmware or a combination of hardware, software and firmware. The waveform generator 320 performs waveform synthesis with a waveform look-up table ("LUT") 410, a waveform shaper 420 and a waveform splitter 430. The waveform LUT 410 is advantageously a memory device, such as a ROM (read only memory) that contains samples of one or more waveform portions or segments containing a single waveform. These stored waveform segments may be as simple as a single period of a triangular waveform, having a sawtooth or symmetric triangle shape, or more complicated, such as a simulated plethysmographic pulse having various physiological features, for example rise time, fall time and dicrotic notch.

The waveform shaper 420 creates a continuous pulsed waveform from the waveform segments provided by the waveform LUT 410. The waveform shaper 420 has a shape parameter input 422 and an event indicator input 424 that are buffered 470 from the parameters 318 output from the internal pulse oximeter 310 (FIG. 3). The shape parameter input 422 determines a particular waveform segment in the waveform LUT 410. The chosen waveform segment is specified by the first address transmitted to the waveform LUT 410 on the address lines 426. The selected waveform segment is sent to the waveform shaper 420 as a series of samples on the waveform data lines 412.

The event indicator input **424** specifies the occurrence of pulses in the plethysmograph waveform processed by the internal pulse oximeter **310** (FIG. 3). For example, the event indicator may be a delta time from the occurrence of a previously detected falling pulse edge or this indicator could be a real time or near real time indicator of the pulse occurrence. The waveform shaper **420** accesses the waveform LUT **410** in a manner to create a corresponding delta time between pulses in the synthesized waveform output **428**. In one embodiment, the waveform shaper is clocked at a predetermined sample rate. From a known number of samples per stored waveform segment and the input delta time from the event indicator, the waveform shaper **420** determines the number of sequential addresses to skip between samples and accesses the waveform LUT **410** accordingly. This effectively "stretches" or "shrinks" the retrieved waveform segment so as to fit in the time between two consecutive pulses detected by the UPO.

The waveform splitter **430** creates a first waveform **432** corresponding to a first waveform (such as a red wavelength) expected by the external pulse oximeter **260** (Fig. 3) and a second waveform (such as infrared) **434** expected by the external pulse oximeter **260**. The relative amplitudes of the first waveform **432** and second waveform **434** are adjusted to correspond to the ratio output **444** from a calibration curve LUT **440**. Thus, for every value of measured oxygen saturation at the sat input **442**, the calibration curve LUT **440** provides a corresponding ratio output **444** that results in the first waveform **432** and the second waveform **434** having an amplitude ratio that will be computed by the external pulse oximeter **260** (FIG. 3) as equivalent to the oxygen saturation measured by the internal pulse oximeter **310** (FIG. 3).

As described above, one particularly advantageous aspect of the UPO is that the operating wavelengths of the sensor **110** (FIG. 3) are not relevant to the operating wavelengths required by the external pulse oximeter **260** (FIG. 3), i.e. the operating wavelengths that correspond to the calibration curve or curves utilized by the external pulse oximeter. The calibration curve LUT **440** simply permits generation of a synthesized waveform as expected by the external oximeter **260** (FIG. 3) based on the calibration curve used by the external pulse oximeter **260** (FIG. 3). The calibration curve LUT **440** contains data about the known calibration curve of the external pulse oximeter **260** (FIG. 3), as specified by the monitor ID input **328**. In other words, the waveform actually synthesized is not a patient plethysmographic waveform. It is merely a stored waveform that will cause the external pulse oximeter to calculate the proper oxygen saturation value and pulse rate values.. Although this does not provide a patient plethysmograph on the external pulse oximeter for the clinician, the calculated values, which is what is actually sought, will be accurate.

A modulator **450** responds to an LED drive input **322** to generate a modulated waveform output **324** derived from the first waveform **432** and second waveform **434**. Also, a data communication interface **460** transmits as a digital data output **326** the data obtained from the sat **442**, pulse rate **462** and synthesized waveform **428** inputs.

FIG. 5 depicts a handheld UPO **500** embodiment. The handheld UPO **500** has keypad inputs **510**, an LCD display **520**, an external power supply input **530**, an output port **540** for connection to an external pulse oximeter and a sensor input **550** at the top edge (not visible). The display **520** shows the measured oxygen saturation **522**, the measured pulse rate **524**, a pulsating bar **526** synchronized with pulse rate or pulse events, and a confidence bar **528**

indicating confidence in the measured values of saturation and pulse rate. Also shown are low battery **572** and alarm enabled **574** status indicators.

The handheld embodiment described in connection with FIG. 5 may also advantageously function in conjunction with a docking station that mechanically accepts, and electrically connects to, the handheld unit. The docking station may be co-located with a patient monitoring system and connected to a corresponding SpO<sub>2</sub> module sensor port, external power supply, printer and telemetry device, to name a few options. In this configuration, the handheld UPO may be removed from a first docking station at one location to accompany and continuously monitor a patient during transport to a second location. The handheld UPO can then be conveniently placed into a second docking station upon arrival at the second location, where the UPO measurements are displayed on the patient monitoring system at that location.

FIG. 6 shows a block diagram of a UPO embodiment, where the functions of the UPO **210** are split between a portable pulse oximeter **610** and a docking station **660**. The portable pulse oximeter **610** ("portable") is a battery operated, fully functional, stand-alone pulse oximeter instrument. The portable **610** connects to a sensor **110** (FIG. 2) through a UPO patient cable **220** (FIG. 2) attached to a patient cable connector **618**. The portable **610** provides the sensor **110** with a drive signal **612** that alternately activates the sensor's red and IR LEDs, as is well-known in the art. The portable also receives a corresponding detector signal **614** from the sensor. The portable can also input a sensor ID on the drive signal line **612**, as described in U.S. Patent No. 5,758,644 entitled Manual and Automatic Probe Calibration, assigned to the assignee of the present invention and incorporated herein by reference.

The portable **610** can be installed into the docking station **660** to expand its functionality. When installed, the portable **610** can receive power **662** from the docking station **660** if the docking station **660** is connected to external power **668**. Alternately, with no external power **668** to the docking station **660**, the portable **610** can supply power **662** to the docking station **660**. The portable **610** communicates to the docking station with a bi-directional serial data line **664**. In particular, the portable **610** provides the docking station with SpO<sub>2</sub>, pulse rate and related parameters computed from the sensor detector signal **614**. When the portable **610** is installed, the docking station **660** may drive a host instrument **260** (FIG. 2) external to the portable **610**. Alternatively, the portable **610** and docking station **660** combination may function as a standalone pulse oximeter instrument, as described below with respect to FIG. 13.

In one embodiment, the docking station **660** does not perform any action when the portable **610** is not docked. The user interface for the docking station **660**, i.e. keypad and display, is on the portable **610**. An indicator LED on the docking station **660** is lit when the portable is docked. The docking station **660** generates a detector signal output **674** to the host instrument **260** (FIG. 2) in response to LED drive signals **672** from the host instrument and SpO<sub>2</sub> values and related parameters received from the portable **610**. The docking station **660** also provides a serial data output **682**, a nurse call **684** and an analog output **688**.

An interface cable **690** connects the docking station **660** to the host instrument patient cable **230** (FIG. 2). The LED drive signals **672** and detector signal output **674** are communicated between the docking station **660** and the

host instrument **260** (FIG. 2) via the interface cable **690**. The interface cable **690** provides a sync data output **692** to the docking station **660**, communicating sensor, host instrument (e.g. monitor ID **328**, FIG. 3) and calibration curve data. Advantageously, this data allows the docking station **660** to appear to a particular host instrument as a particular sensor providing patient measurements.

5           FIG. 7 provides further detail of the portable **610**. The portable components include a pulse oximeter processor **710**, a management processor **720**, a power supply **730**, a display **740** and a keypad **750**. The pulse oximeter processor **710** functions as an internal pulse oximeter, interfacing the portable to a sensor **110** (FIG. 2) and deriving SpO<sub>2</sub>, pulse rate, a plethysmograph and a pulse indicator. An advanced pulse oximeter for use as the pulse oximeter processor **710** is described in U.S. Patent No. 5,632,272, referenced above. An advanced pulse oximetry sensor  
10           for use as the sensor **110** (FIG. 2) attached to the pulse oximeter processor **710** is described in U.S. Patent No. 5,638,818, also referenced above. Further, a line of advanced Masimo SET<sup>®</sup> pulse oximeter OEM boards and sensors are available from the assignee of the present invention. In one embodiment, the pulse oximeter processor **710** is the Masimo SET<sup>®</sup> MS-3L board or a low power MS-5 board.

          The management processor **720** controls the various functions of the portable **610**, including asynchronous  
15           serial data communications **724** with the pulse oximeter processor **710** and synchronous serial communications **762** with the docking station **660** (FIG. 6). The physical and electrical connection to the docking station **660** (FIG. 6) is via a docking station connector **763** and the docking station interface **760**, respectively. The processor **720** utilizes a real-time clock **702** to keep the current date and time, which includes time and date information that is stored along with SpO<sub>2</sub> parameters to create trend data. The processor of the portable **610** and the docking station **660** (FIG. 6)  
20           can be from the same family to share common routines and minimize code development time.

          The processor **720** also controls the user interface **800** (FIG. 8A) by transferring data **742** to the display  
          **740**, including display updates and visual alarms, and by interpreting keystroke data **752** from the keypad **750**. The processor **720** generates various alarm signals, when required, via an enable signal **728**, which controls a speaker driver **770**. The speaker driver **770** actuates a speaker **772**, which provides audible indications such as, for example,  
25           alarms and pulse beeps. The processor **720** also monitors system status, which includes battery status **736**, indicating battery levels, and docked status **764**, indicating whether the portable **610** is connected to the docking station **660** (FIG. 6). When the portable **610** is docked and is on, the processor **720** also decides when to turn on or off docking station power **732**.

          Advantageously, the caregiver can set (i.e. configure or program) the behavior of the portable display **740** and  
30           alarms when the docked portable **610** senses that an interface cable **690** has connected the docking station **660** to an external pulse oximeter, such as a multiparameter patient monitoring system. In one user setting, for example, the portable display **740** stops showing the SpO<sub>2</sub> **811** (FIG. 8) and pulse rate **813** (FIG. 8) values when connected to an external pulse oximeter to avoid confusing the caregiver, who can read equivalent values on the patient monitoring system. The display **740**, however, continues to show the plethysmograph **815** (FIG. 8) and visual pulse indicator **817**  
35           (FIG. 8) waveforms. For one such user setting, the portable alarms remain active.

Another task of the processor **720** includes maintenance of a watchdog function. The watchdog **780** monitors processor status on the watchdog data input **782** and asserts the  $\mu$ P reset output **784** if a fault is detected. This resets the management processor **720**, and the fault is indicated with audible and visual alarms.

The portable **610** gets its power from batteries in the power supply **730** or from power **766** supplied from the docking station **660** (FIG. 6) via the docking station interface **760**. A power manager **790** monitors the on/off switch on the keypad **750** and turns-on the portable power accordingly. The power manager **790** turns off the portable on command by the processor **720**. DC/DC converters within the power supply **730** generate the required voltages **738** for operation of the portable **610** and docking station power **732**. The portable batteries can be either alkaline rechargeable batteries or another renewable power source. The batteries of the power supply **730** supply docking station power **732** when the docking station **660** (FIG. 6) is without external power. A battery charger within the docking station power supply provides charging current **768** to rechargeable batteries within the power supply **730**. The docking station power supply **990** (FIG. 9) monitors temperature **734** from a thermistor in the rechargeable battery pack, providing an indication of battery charge status.

A non-volatile memory **706** is connected to the management processor **720** via a high-speed bus **722**. In the present embodiment, the memory **706** is an erasable and field re-programmable device used to store boot data, manufacturing serial numbers, diagnostic failure history, adult SpO<sub>2</sub> and pulse rate alarm limits, neonate SpO<sub>2</sub> and pulse rate alarm limits, SpO<sub>2</sub> and pulse rate trend data, and program data. Other types of non-volatile memory are well known. The SpO<sub>2</sub> and pulse rate alarm limits, as well as SpO<sub>2</sub> related algorithm parameters, may be automatically selected based on the type of sensor **110** (FIG. 2), adult or neonate, connected to the portable **610**.

The LCD display **740** employs LEDs for a backlight to increase its contrast ratio and viewing distance when in a dark environment. The intensity of the backlight is determined by the power source for the portable **610**. When the portable **610** is powered by either a battery pack within its power supply **730** or a battery pack in the docking station power supply **990** (FIG. 9), the backlight intensity is at a minimum level. When the portable **610** is powered by external power **668** (FIG. 6), the backlight is at a higher intensity to increase viewing distance and angle. In one embodiment, button on the portable permits overriding these intensity settings, and provides adjustment of the intensity. The backlight is controlled in two ways. Whenever any key is pressed, the backlight is illuminated for a fixed number of seconds and then turns off, except when the portable is docked and derives power from an external source. In that case, the backlight is normally on unless deactivated with a key on the portable **610**.

FIG. 8A illustrates the portable user interface **800**, which includes a display **740** and a keypad **750**. In one embodiment, the display **740** is a dot matrix LCD device having 160 pixels by 480 pixels. The display **740** can be shown in portrait mode, illustrated in FIG. 8B, or in landscape mode, illustrated in FIG. 8C. A tilt sensor **950** (FIG. 9) in the docking station **660** (FIG. 6) or a display mode key on the portable **610** (FIG. 6) determines portrait or landscape mode. The tilt sensor **950** (FIG. 9) can be a gravity-activated switch or other device responsive to orientation and can be alternatively located in the portable **610** (FIG. 6). In a particular embodiment, the tilt sensor **950** (FIG. 9) is a non-

mercury tilt switch, part number CW 1300-1, available from Comus International, Nutley, NJ (www.comus-intl.com). The tilt sensor **950** (FIG. 9) could also be a mercury tilt switch.

Examples of how the display area can be used to display  $\text{SpO}_2$  **811**, pulse rate **813**, a plethysmographic waveform **815**, a visual pulse indicator **817** and soft key icons **820** in portrait and landscape mode are shown in FIGS. **8B** and **8C**, respectively. The software program of the management processor **720** (FIG. 7) can be easily changed to modify the category, layout and size of the display information shown in FIGS. **8B-C**. Other advantageous information for display is  $\text{SpO}_2$  limits, alarm, alarm disabled, exception messages and battery status.

The keypad **750** includes soft keys **870** and fixed keys **880**. The fixed keys **880** each have a fixed function. The soft keys **870** each have a function that is programmable and indicated by one of the soft key icons **820** located next to the soft keys **870**. That is, a particular one of the soft key icons **820** is in proximity to a particular one of the soft keys **870** and has a text or a shape that suggests the function of that particular one of the soft keys **870**. In one embodiment, the button portion of each key of the keypad **750** is constructed of florescent material so that the keys **870**, **880** are readily visible in the dark.

In one embodiment, the keypad **750** has one row of four soft keys **870** and one row of three fixed keys **880**. Other configurations are, of course, available, and specific arrangement is not significant. The functions of the three fixed keys **880** are power, alarm silence and light/contrast. The power function is an on/off toggle button. The alarm silence function and the light/contrast function have dual purposes depending on the duration of the key press. A momentary press of the key corresponding to the alarm silence function will disable the audible alarm for a fixed period of time. To disable the audible alarm indefinitely, the key corresponding to the alarm silence function is held down for a specified length of time. If the key corresponding to the alarm silence function is pressed while the audible alarm has been silenced, the audible alarm is reactivated. If the key corresponding to the light/contrast function is pressed momentarily, it is an on/off toggle button for the backlight. If the key corresponding to the light/contrast function is held down, the display contrast cycles through its possible values.

In this embodiment, the default functions of the four soft keys **870** are pulse beep up volume, pulse beep down volume, menu select, and display mode. These functions are indicated on the display by the up arrow, down arrow, "menu" and curved arrow soft key icons **820**, respectively. The up volume and down volume functions increase or decrease the audible sound or "beep" associated with each detected pulse. The display mode function rotates the display **740** through all four orthogonal orientations, including portrait mode (FIG. **8B**) and landscape mode (FIG. **8C**), with each press of the corresponding key. The menu select function allows the functionality of the soft keys **870** to change from the default functions described above. Examples of additional soft key functions that can be selected using this menu feature are set  $\text{SpO}_2$  high/low limit, set pulse rate high/low limit, set alarm volume levels, set display to show trend data, print trend data, erase trend data, set averaging time, set sensitivity mode, perform synchronization, perform rechargeable battery maintenance (deep discharge/recharge to remove battery memory), and display product version number.

FIG. 9 provides further details of the docking station 660, which includes a docking station processor 910, a non-volatile memory 920, a waveform generator 930, a PROM interface 940, a tilt sensor 950, a portable interface 970 and associated connector 972, status indicators 982, a serial data port 682, a nurse call output 684, an analog output 688 and a power supply 990. In one embodiment, the docking station 660 is intended to be associated with a fixed (non-transportable) host instrument, such as a multiparameter patient monitoring instrument in a hospital emergency room. In a transportable embodiment, the docking station 660 is movable, and includes a battery pack within the power supply 990.

The docking station processor 910 orchestrates the activity on the docking station 660. The processor 910 provides the waveform generator 930 with parameters 932 as discussed above for Figures 3 and 4. The processor 910 also provides asynchronous serial data 912 for communications with external devices and synchronous serial data 971 for communications with the portable 610 (FIG. 6). In addition, the processor 910 determines system status including sync status 942, tilt status 952 and power status 992. The portable management processor 720 (FIG. 7) performs the watchdog function for the docking station processor 910. The docking station processor 910 sends watchdog messages to the portable processor 720 (FIG. 7) as part of the synchronous serial data 972 to ensure the correct operation of the docking station processor 910.

The docking station processor 910 accesses non-volatile memory 920 over a high-speed bus 922. The non-volatile memory 920 is re-programmable and contains program data for the processor 910 including instrument communication protocols, synchronization information, a boot image, manufacturing history and diagnostic failure history.

The waveform generator 930 generates a synthesized waveform that a conventional pulse oximeter can process to calculate SpO<sub>2</sub> and pulse rate values or exception messages, as described above with respect to FIG. 4. However, in the present embodiment, as explained above, the waveform generator output does not reflect a physiological waveform. It is merely a waveform constructed to cause the external pulse oximeter to calculate the correct saturation and pulse rate.. In an alternative embodiment, physiological data could be provided to the external pulse oximeter, but the external pulse oximeter would generally not be able to calculate the proper saturation values, and the upgrading feature would be lost. The waveform generator 930 is enabled if an interface cable 690 (FIG. 6), described below with respect to FIG. 10, with valid synchronization information is connected. Otherwise, the power to the waveform generator 930 is disabled.

The status indicators 982 are a set of LEDs on the front of the docking station 660 used to indicate various conditions including external power (AC), portable docked, portable battery charging, docking station battery charging and alarm. The serial data port 682 is used to interface with either a computer, a serial port of conventional pulse oximeters or serial printers via a standard RS-232 DB-9 connector 962. This port 682 can output trend memory, SpO<sub>2</sub> and pulse rate and support the system protocols of various manufacturers. The analog output 688 is used to interface with analog input chart recorders via a connector 964 and can output "real-time" or trend SpO<sub>2</sub> and pulse rate data. The nurse call output 684 from a connector 964 is activated when alarm limits are exceeded for a predetermined

number of consecutive seconds. In another embodiment, data, including alarms, could be routed to any number of communications ports, and even over the Internet, to permit remote use of the upgrading pulse oximeter.

The PROM interface **940** accesses synchronization data **692** from the PROM **1010** (FIG. **10**) in the interface cable **690** (FIGS. **6**, **10**) and provides synchronization status **942** to the docking station processor **910**. The portable interface **970** provides the interconnection to the portable **610** (FIG. **6**) through the docking station interface **760** (FIG. **7**).

As shown in FIG. **9**, external power **668** is provided to the docking station **660** through a standard AC connector **968** and on/off switch **969**. When the docking station **660** has external power **668**, the power supply **990** charges the battery in the portable power supply **730** (FIG. **7**) and the battery, if any, in the docking station power supply **990**. When the portable **610** (FIG. **6**) is either removed or turned off, the docking station power **973** is removed and the docking station **660** is turned off, except for the battery charger portion of the power supply **990**. The docking station power **973** and, hence, the docking station **660** turn on whenever a docked portable **610** (FIG. **6**) is turned on. The portable **610** (FIG. **6**) supplies power for an embodiment of the docking station **660** without a battery when external power **668** is removed or fails.

FIG. **10** provides further detail regarding the interface cable **690** used to connect between the docking station **660** (FIG. **6**) and the patient cable **230** (FIG. **2**) of a host instrument **260** (FIG. **2**). The interface cable **690** is configured to interface to a specific host instrument and to appear to the host instrument as a specific sensor. A PROM **1010** built into the interface cable **690** contains information identifying a sensor type, a specific host instrument, and the calibration curve of the specific host instrument. The PROM information can be read by the docking station **660** (FIG. **6**) as synchronization data **692**. Advantageously, the synchronization data **692** allows the docking station **660** (FIG. **6**) to generate a waveform to the host instrument that causes the host instrument to display SpO<sub>2</sub> values equivalent to those calculated by the portable **610** (FIG. **6**). The interface cable **690** includes an LED drive path **672**. In the embodiment shown in FIG. **10**, the LED drive path **672** is configured for common anode LEDs and includes IR cathode, red cathode and common anode signals. The interface cable **690** also includes a detector drive path **674**, including detector anode and detector cathode signals.

A menu option on the portable **610** (FIG. **6**) also allows synchronization information to be calculated in the field. With manual synchronization, the docking station **660** (FIG. **6**) generates a waveform to the host instrument **260** (FIG. **2**) and displays an expected SpO<sub>2</sub> value. The user enters the SpO<sub>2</sub> value displayed on the host instrument using the portable keypad **750** (FIG. **7**). These steps are repeated until a predetermined number of data points are entered and the SpO<sub>2</sub> values displayed by the portable and the host instrument are consistent.

FIGS. **11A-B** depict an embodiment of the portable **610**, as described above with respect to FIG. **6**. FIGS. **12A-B** depict an embodiment of the docking station **660**, as described above with respect to FIG. **6**. FIG. **13** depicts an embodiment of the UPO **210** where the portable **610** is docked with the docking station **660**, also as described above with respect to FIG. **6**.



FIG. 11A depicts the portable front panel 1110. The portable 610 has a patient cable connector 618, as described above with respect to FIG. 6. Advantageously, the connector 618 is rotatably mounted so as to minimize stress on an attached patient cable (not shown). In one embodiment, the connector 618 can freely swivel between a plane parallel to the front panel 1110 and a plane parallel to the side panel 1130. In another embodiment, the connector 618 can swivel between, and be releasably retained in, three locked positions. A first locked position is as shown, where the connector is in a plane parallel to the front panel 1110. A second locked position is where the connector 618 is in a plane parallel to the side panel 1130. The connector 618 also has an intermediate locked position 45° between the first and the second locked positions. The connector 618 is placed in the first locked position for attachment to the docking station 660.

Shown in FIG. 11A, the portable front panel 1110 also has a speaker 772, as described with respect to FIG. 7. Further, the front panel 1110 has a row of soft keys 870 and fixed keys 880, as described above with respect to FIG. 8. In addition, the front panel 1110 has a finger actuated latch 1120 that locks onto a corresponding catch 1244 (FIG. 12A) in the docking station 660, allowing the portable 610 to be releasably retained by the docking station 660. An OEM label can be affixed to a recessed area 1112 on the front panel 1110.

FIG. 11B depicts the portable back panel 1140. The back panel 1140 has a socket 763, a pole clamp mating surface 1160, and a battery pack compartment 1170. The socket 763 is configured to mate with a corresponding docking station plug 972 (FIG. 12A). The socket 763 and plug 972 (FIG. 12A) provide the electrical connection interface between the portable 610 and the docking station 660 (FIG. 12A). The socket 763 houses multiple spring contacts that compress against plated edge-connector portions of the docking station plug 972 (FIG. 12A). A conventional pole clamp (not shown) may be removably attached to the mating surface 1160. This conveniently allows the portable 610 to be held to various patient-side or bedside mounts for hands-free pulse oximetry monitoring. The portable power supply 730 (FIG. 7) is contained within the battery pack compartment 1170. The compartment 1170 has a removable cover 1172 for protection, insertion and removal of the portable battery pack. Product labels, such as a serial number identifying a particular portable, can be affixed with the back panel indent 1142.

FIG. 12A depicts the front side 1210 of the docking station 660. The front side 1210 has a docking compartment 1220, a pole clamp recess 1230, pivots 1242, a catch 1244, a plug connector 972 and LED status indicators 982. The docking compartment 1220 accepts and retains the portable 610 (FIGS. 11A-B), as shown in FIG. 13. When the portable 610 (FIGS. 11A-B) is docked in the compartment 1220, the pole clamp recess 1230 accommodates a pole clamp (not shown) attached to the portable's pole clamp mating surface 1160 (FIG. 11B), assuming the pole clamp is in its closed position. The portable 610 (FIGS. 11A-B) is retained in the compartment 1220 by pivots 1242 that fit into corresponding holes in the portable's side face 1130 and a catch 1244 that engages the portable's latch 1120 (FIG. 11A). Thus, the portable 610 (FIGS. 11A-B) is docked by first attaching it at one end to the pivots 1242, then rotating it about the pivots 1242 into the compartment 1220, where it is latched in place on the catch 1244. The portable 610 (FIGS. 11A-B) is undocked in reverse order, by first pressing the latch

1120 (FIG. 11A), which releases the portable from the catch 1244, rotating the portable 610 (FIGS. 11A-B) about the pivots 1242 out of the compartment 1220 and then removing it from the pivots 1242. As the portable is rotated into the compartment, the docking station plug 972 inserts into the portable socket 763 (FIG. 11B), providing the electrical interface between the portable 610 and the docking station 660. The status indicators 982 are as described above with respect to FIG. 9.

FIG. 12B depicts the back side 1260 of the docking station 660. The back side 1260 has a serial (RS-232 or USB) connector 962, an analog output and nurse call connector 964, an upgrade port connector 966, an AC power plug 968, an on/off switch 969 and a ground lug 1162. A handle 1180 is provided at one end and fan vents 1170 are provided at the opposite end. A pair of feet 1190 are visible near the back side 1260. A corresponding pair of feet (not visible) are located near the front side 1210 (FIG. 12A). The feet near the front side 1210 extend so as to tilt the front side 1210 (FIG. 12A) upward, making the display 740 (FIG. 13) of a docked portable 610 (FIG. 13) easier to read.

FIG. 13 illustrates both the portable 610 and the docking station 660. The portable 610 and docking station 660 constitute three distinct pulse oximetry instruments. First, the portable 610 by itself, as depicted in FIGS. 11A-B, is a handheld pulse oximeter applicable to various patient monitoring tasks requiring battery power or significant mobility, such as ambulance and ER situations. Second, the portable 610 docked in the docking station 660, as depicted in FIG. 13, is a standalone pulse oximeter applicable to a wide-range of typical patient monitoring situations from hospital room to the operating room. Third, the portable 610 docked and the upgrade port 966 (FIG. 12B) connected with an interface cable to the sensor port of a conventional pulse oximeter module 268 (FIG. 2) within a multiparameter patient monitoring instrument 260 (FIG. 2) or other conventional pulse oximeter, is a universal/upgrading pulse oximeter (UPO) instrument 210, as described herein. Thus, the portable 610 and docking station 660 configuration of the UPO 210 advantageously provides a three-in-one pulse oximetry instrument functionality.

Another embodiment of the docking station 660 incorporates an input port that connects to a blood pressure sensor and an output port that connects to the blood pressure sensor port of a multiparameter patient monitoring system (MPMS). The docking station 660 incorporates a signal processor that computes a blood pressure measurement based upon an input from the blood pressure sensor. The docking station 660 also incorporates a waveform generator connected to the output port that produces a synthesized waveform based upon the computed measurement. The waveform generator output is adjustable so that the blood pressure value displayed on the MPMS is equivalent to the computed blood pressure measurement. Further, when the portable 610 is docked in the docking station 660 and the blood pressure sensor is connected to the input port, the portable displays a blood pressure value according to the computed blood pressure measurement. Thus, in this embodiment, the docking station 660 provides universal/upgrading capability for both blood pressure and SpO<sub>2</sub>.

Likewise, the docking station 660 can function as an universal/upgrading instrument for other vital sign measurements, such as respiratory rate, EKG or EEG. For this embodiment, the docking station 660 incorporates

related sensor connectors and associated sensor signal processors and upgrade connectors to an MPMS or standalone instrument. In this manner, a variety of vital sign measurements can be incorporated into the docking station **660**, either individually or in combination, with or without  $\text{SpO}_2$  as a measurement parameter, and with or without the portable **610**. In yet another embodiment, the docking station **660** can be configured as a simple  $\text{SpO}_2$  upgrade box, incorporating a  $\text{SpO}_2$  processor and patient cable connector for a  $\text{SpO}_2$  sensor that functions with or without the portable **610**.

Unlike a conventional standalone pulse oximeter, the standalone configuration shown in FIG. **13** has a rotatable display **740** that allows the instrument to be operated in either a vertical or horizontal orientation. A tilt sensor **950** (FIG. **9**) indicates when the bottom face **1310** is placed along a horizontal surface or is otherwise horizontally-oriented. In this horizontal orientation, the display **740** appears in landscape mode (FIG. **8C**). The tilt sensor **950** (FIG. **9**) also indicates when the side face **1320** is placed along a horizontal surface or is otherwise horizontally oriented. In this vertical orientation, the display **740** appears in portrait mode (FIG. **8B**). A soft key **870** on the portable **610** can override the tilt sensor, allowing the display to be presented at any  $90^\circ$  orientation, i.e. portrait, landscape, "upside-down" portrait or "upside-down" landscape orientations. The handheld configuration (FIG. **11A**), can also present the display **740** at any  $90^\circ$  orientation using a soft key **870**. In the particular embodiment described above, however, the portable **610** does not have a tilt sensor and, hence, relies on a soft key **870** to change the orientation of the display when not docked.

FIG. **14** illustrates the docking station **660** incorporated within a local area network (LAN). The LAN shown is Ethernet-based **1460**, using a central LAN server **1420** to interconnect various LAN clients **1430** and other system resources such as printers and storage (not shown). An Ethernet controller module **1410** is incorporated with the docking station **660**. The controller module **1410** can be incorporated within the docking station **660** housing or constructed as an external unit. In this manner, the UPO, according to the present invention, can communicate with other devices on the LAN or over the Internet **1490**.

The Ethernet controller module **1410** can be embedded with web server firmware, such as the Hewlett-Packard (HP) BFOOT-10501. The module **1410** has both a 10 Base-T Ethernet interface for connection to the Ethernet **1460** and a serial interface, such as RS-232 or USB, for connection to the docking station **660**. The module firmware incorporates HTTP and TCP/IP protocols for standard communications over the World Wide Web. The firmware also incorporates a micro web server that allows custom web pages to be served to remote clients over the Internet, for example. Custom C++ programming allows expanded capabilities such as data reduction, event detection and dynamic web page configuration.

As shown in FIG. **14**, there are many applications for the docking station **660** to Ethernet interface. Multiple UPOs can be connected to a hospital's LAN, and a computer on the LAN could be utilized to upload pulse rate and saturation data from the various UPOs, displaying the results. Thus, this Ethernet interface could be used to implement a central pulse oximetry monitoring station within a hospital. Further, multiple UPOs from anywhere in the world can be monitored from a central location via the Internet. Each UPO is addressable as an individual web site and

downloads web pages viewable on a standard browser, the web pages displaying oxygen saturation, pulse rate and related physiological measurements from the UPO. This feature allows a caregiver to monitor a patient regardless of where the patient or caregiver is located. For example a caregiver located at home in one city or at a particular hospital could download measurements from a patient located at home in a different city or at the same or a different hospital. Other applications include troubleshooting newly installed UPOs or uploading software patches or upgrades to UPOs via the Internet. In addition alarms could be forwarded to the URL of the clinician monitoring the patient.

The UPO may have other configurations besides the handheld unit described in connection with FIG. 5 or the portable 610 and docking station 660 combination described in connection with FIGS. 11-13. The UPO may be a module, with or without a display, that can be removably fastened to a patient via an arm strap, necklace or similar means. In a smaller embodiment, this UPO module may be integrated into a cable or connector used for attaching a sensor to a pulse oximeter. The UPO may also be a circuit card or module that can externally or internally plug into or mate with a standalone pulse oximeter or multiparameter patient monitoring system. Alternatively, the UPO may be configured as a simple standalone upgrade instrument.

Further, although a universal/upgrading apparatus and method have been mainly described in terms of a pulse oximetry measurement embodiment, the present invention is equally applicable to other physiological measurement parameters such as blood pressure, respiration rate, EEG and ECG, to name a few. In addition, a universal/upgrading instrument having a single physiological measurement parameter or a multiple measurement parameter capability and configured as a handheld, standalone, portable, docking station, module, plug-in, circuit card, to name a few, is also within the scope of the present invention.

The UPO has been disclosed in detail in connection with various embodiments of the present invention. These embodiments are disclosed by way of examples only and are not to limit the scope of the present invention, which is defined by the claims that follow. One of ordinary skill in the art will appreciate many variations and modifications within the scope of this invention.

WHAT IS CLAIMED IS:

1. A measurement apparatus comprising:

a sensor having at least one emitter and an associated detector configured to attach to a tissue site, said detector providing a detector signal responsive to the intensity of energy from said emitter after it has passed through said tissue site;

a first pulse oximeter in communication with said detector and configured to compute an oxygen saturation measurement based on said detector signal;

a waveform generator responsive to said oxygen saturation measurement to generate at least one generated waveform based on said oxygen saturation measurement, wherein said at least one waveform is synthesized so that a second pulse oximeter receiving said waveform would calculate an oxygen saturation value generally equivalent to said oxygen saturation measurement.

2. The measurement apparatus of Claim 1 wherein said at least one waveform comprises a first waveform and a second waveform, where the amplitude ratio of said first and second waveforms are selected so that said oxygen saturation value is generally equivalent to said oxygen saturation measurement.

3. The measurement apparatus of Claim 2, wherein said first and second waveforms are generated from a look-up table.

4. The measurement apparatus of Claim 3, wherein said first and second waveforms are triangular.

5. The measurement apparatus of Claim 1, wherein said first pulse oximeter further computes a pulse rate measurement based on said detector signal, said generated waveform based in part on said pulse rate measurement in a manner such that said second pulse oximeter receiving said generated waveform would calculate a pulse rate value generally equivalent to said pulse rate measurement.

6. The measurement apparatus of Claim 1 further comprising:

a portable portion comprising said first pulse oximeter; and

a docking station portion comprising said waveform generator, wherein said portable portion is removably attached and in communication with said docking station portion when said portable portion is attached to said docking station portion.

7. The measurement apparatus of Claim 6 further comprising:

a display mounted on said portable portion.

8. The measurement apparatus of Claim 7, further comprising a tilt sensor located, wherein the mode of said display is determined by the output of said tilt sensor.

9. The measurement apparatus of Claim 8, wherein said tilt-sensor is provided by said docking station portion.

10. The measurement apparatus of Claim 9, wherein an image on said display is oriented in response to said tilt sensor.

11. The measurement apparatus of Claim 7, wherein an image on said display is rotatable in orientation with respect to said display in 90 degree increments.

12. A measurement apparatus comprising:

a first sensor port connectable to a sensor;

an upgrade port connectable to a second sensor port of an external measurement apparatus;

a signal processor that computes a measurement based on a signal input to said first sensor port;

a signal generator responsive to said measurement to produce a synthesized signal, said synthesized signal being provided to said upgrade port, wherein said synthesized signal is generated such that said external measurement apparatus will calculate a value generally equivalent to said measurement when said upgrade port is attached to said second sensor port.

13. The measurement apparatus of Claim 12 wherein said sensor is generally incompatible with said second sensor port.

14. The measurement apparatus of Claim 12 wherein said signal processor is an improved measurement apparatus from said external measurement apparatus.

15. The measurement apparatus of Claim 12, wherein said measurement apparatus is a physiological monitor which calculates a physiological parameter, and wherein said external measurement apparatus is a physiological monitor which capable of calculating said physiological parameter.

16. A measurement method comprising the steps of:

obtaining an intensity signal responsive to the oxygen content of blood at a tissue site;

computing an oxygen saturation measurement based on said intensity signal; and

generating a waveform based on said oxygen saturation measurement, wherein said waveform is configured to cause a pulse oximeter receiving said waveform to calculate an oxygen saturation value generally equivalent to said oxygen saturation measurement.

17. The method of Claim 16, further comprising providing said waveform to the sensor inputs of an pulse oximeter.

18. The measurement method of Claim 17 wherein said generating step comprises:

reading waveform values from a waveform lookup table;

creating a first set of waveform data and a second set of waveform data based on said waveform values;

and

combining portions of said first set and said second set of waveform data into a set of modulated waveform data configured to be provided to said pulse oximeter.

19. The measurement method of Claim 16 wherein said generating step further comprises:

inputting said oxygen saturation measurement to a calibration curve lookup table;

outputting a ratio from said calibration curve lookup table; and

adjusting said second set of waveform data to correlate to said ratio.

20. The measurement method of Claim 16 further comprising:  
determining a pulse rate measurement based on said intensity signal; and  
adjusting the sample rate of said waveform so that said waveform is configured configured to cause said  
pulse oximeter receiving said waveform to display a pulse rate value generally equivalent to said pulse rate  
5 measurement.

21. A measurement method comprising the steps of:  
sensing a physiological signal;  
computing a physiological parameter based upon said signal;  
synthesizing a waveform as a function of said physiological parameter, said synthesizing performed such that  
10 an external physiological monitor receiving said waveform will ascertain a value corresponding to said physiological  
parameter.

22. The method of Claim 21, further comprising outputting said waveform to a sensor input of said  
external physiological monitoring apparatus.

23. The measurement method of Claim 21 further comprising the steps of:  
15 connecting an interface cable to said sensor input, said cable configured to transmit said waveform to said  
physiological monitoring apparatus and to provide a plurality of characterization data for said measurement apparatus;  
and

reading said characterization data from said cable, said synthesizing step being based on said data.

24. The measurement method of Claim 23 wherein said physiological signal is an intensity signal  
20 responsive to the oxygen content of blood at a tissue site and said characterization data is a calibration curve relating  
a set of ratios to a set of oxygen saturation values.

25. A measurement apparatus comprising:  
a first pulse oximeter configured to determine oxygen saturation measurements and pulse rate measurements  
based upon an intensity signal derived from a tissue site;

25 means for creating a waveform signal based upon said oxygen saturation measurement and said pulse rate  
measurements; and

means for transmitting said waveform signal to a second pulse oximeter.

26. The measurement apparatus of Claim 25 further comprising means for calibrating said waveform  
signal so that said second pulse oximeter displays oxygen saturation values generally equivalent to said oxygen  
30 saturation measurements.

27. The measurement apparatus of Claim 25 further comprising means for timing said waveform signal  
so that said second pulse oximeter displays a pulse rate value generally equivalent to said pulse rate measurement.

28. The measurement apparatus of Claim 25 further comprising means for displaying said oxygen  
saturation measurement and said pulse rate measurement on said first pulse oximeter.

29. The measurement apparatus of Claim 28 further comprising means for sensing gravity and for altering an orientation mode of said means for displaying as a function of the orientation of said first pulse oximeter.

30. The measurement apparatus of Claim 28 further comprising means for manually altering an orientation mode of said display means.

5 31. A measurement apparatus comprising:

a portable portion having a sensor port, a processor, and a display, said sensor port configured to receive a signal indicative of a physiological parameter, said processor programmed to compute a physiological parameter measurement based upon said intensity signal and to output said physiological parameter measurement to said display, said portable portion configured to operate as a hand-held physiological monitor;

10 a docking station configured to receive said portable portion and in communication with said portable portion; and

wherein said portable portion has a docked position with said docking station in which the combination of said portable portion and said docking station has at least one function beyond that of said portable portion.

32. The measurement apparatus of Claim 31 wherein said at least one function comprises generating a waveform for an external physiological monitor, said waveform configured to cause said external physiological monitor to display a physiological parameter value generally consistent with the physiological parameter measurement.

33. The measurement apparatus of Claim 32, wherein said physiological parameter measurement is arterial blood oxygen saturation.

34. The measurement apparatus of Claim 31 wherein said at least one function comprises downloading a web page displaying said physiological parameter measurement when said docking station is addressed by a remote Internet client.

35. The measurement apparatus of Claim 31 wherein said portable portion has a key-actuated image rotatable display.

36. The measurement apparatus of Claim 35 wherein said image rotatable display is a function of the orientation of said portable portion when said portable portion is in said docked position.

37. A measurement apparatus configured to function in both a first placement orientation and a second placement orientation, said apparatus comprising:

a tilt sensor providing an output responsive to gravity; and

30 a display having a first mode and a second mode, said display responsive to said tilt sensor to operate in a first mode when said apparatus is in said first placement orientation and in a second mode when said apparatus is in said second placement orientation, said first and second mode controlling the orientation of data on said display.

38. The measurement apparatus of Claim 37, wherein said measurement apparatus is a physiological monitor, said apparatus further comprising:

a sensor port configured to receive a signal responsive to a physiological state; and



a processor in communication with said sensor port and said tilt sensor output, said processor programmed to compute a physiological measurement based upon said signal and to determine whether said measurement apparatus is in said first placement orientation or said second placement orientation based upon said tilt sensor output, and to drive said display in said first mode or said second mode.

5           39.       The measurement apparatus of Claim 38 wherein said signal is a detected light intensity responsive to the attenuation at a tissue site and wherein said physiological measurement value is an oxygen saturation value.

          40.       The measurement apparatus of Claim 37 further comprising a key that, when actuated, changes said display from said first mode to said second mode.

10          41.       The measurement apparatus of Claim 37 wherein said measurement apparatus has a rectangular face with a shorter first edge and a longer second edge, said display forming at least a portion of said face, said first placement orientation being with said first edge aligned generally vertically and said second edge aligned generally horizontally, said first mode providing a landscape presentation for said display.

15          42.       The measurement apparatus of Claim 37 wherein said measurement apparatus has a rectangular face with a shorter first edge and a longer second edge, said display forming at least a portion of said face, said second spatial orientation being with said first edge aligned generally horizontally and said second edge aligned generally vertically, said second mode providing a portrait presentation for said display.

          43.       A measurement method comprising the steps of:

sensing a signal responsive to a physiological state;

computing a physiological measurement based on said signal;

20       determining the spatial orientation of a tilt sensor; and

displaying said physiological measurement in a mode that is based upon said determining step.

          44.       The measurement method of Claim 43 wherein said signal is an intensity signal responsive to attenuation at a tissue site and said physiological measurement is oxygen saturation.

25          45.       The measurement method of Claim 43 wherein said mode comprises a portrait presentation of said physiological measurement.

          46.       The measurement method of Claim 43 wherein said mode comprises a landscape presentation of said physiological measurement.

30          47.       The measurement method of Claim 43 further comprising altering said mode upon the actuation of a key switch.

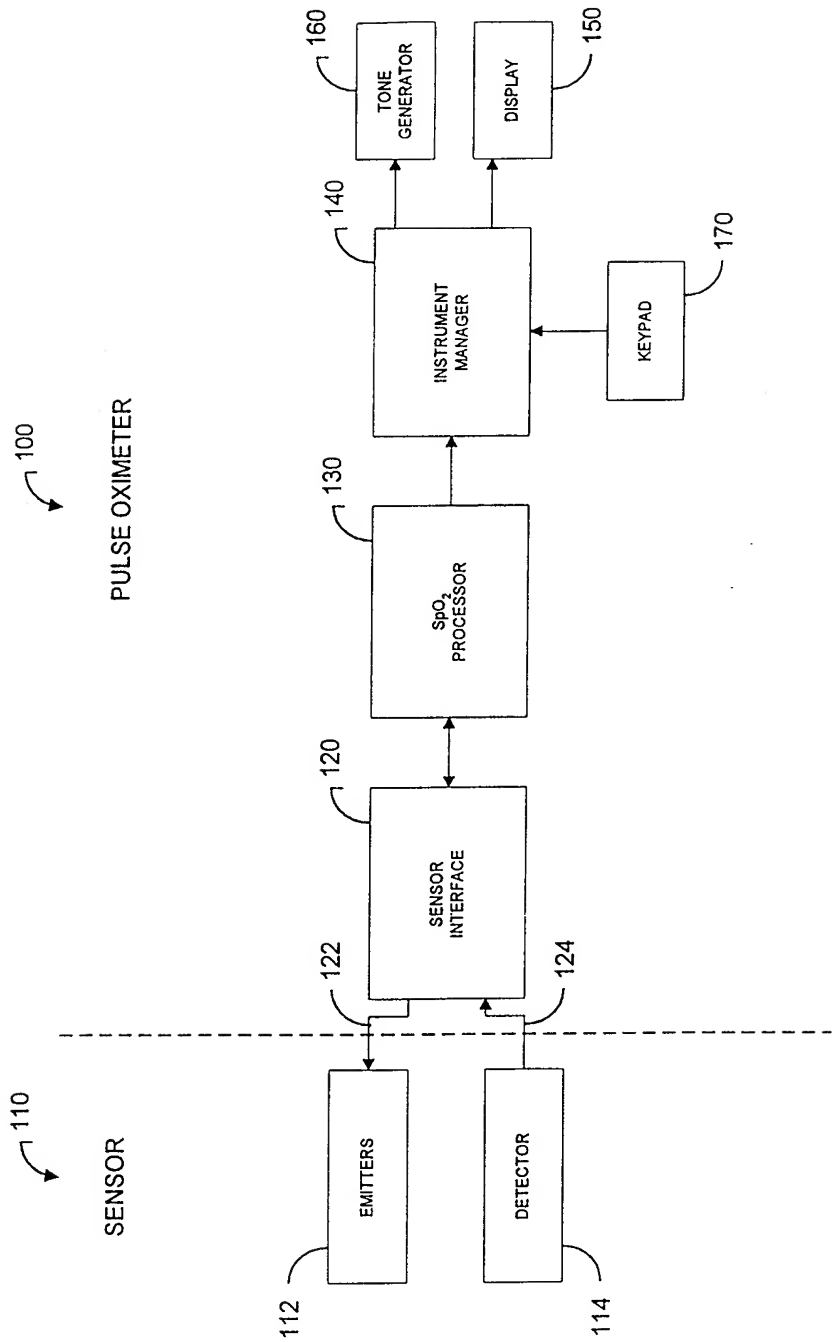


FIG. 1 (prior art)

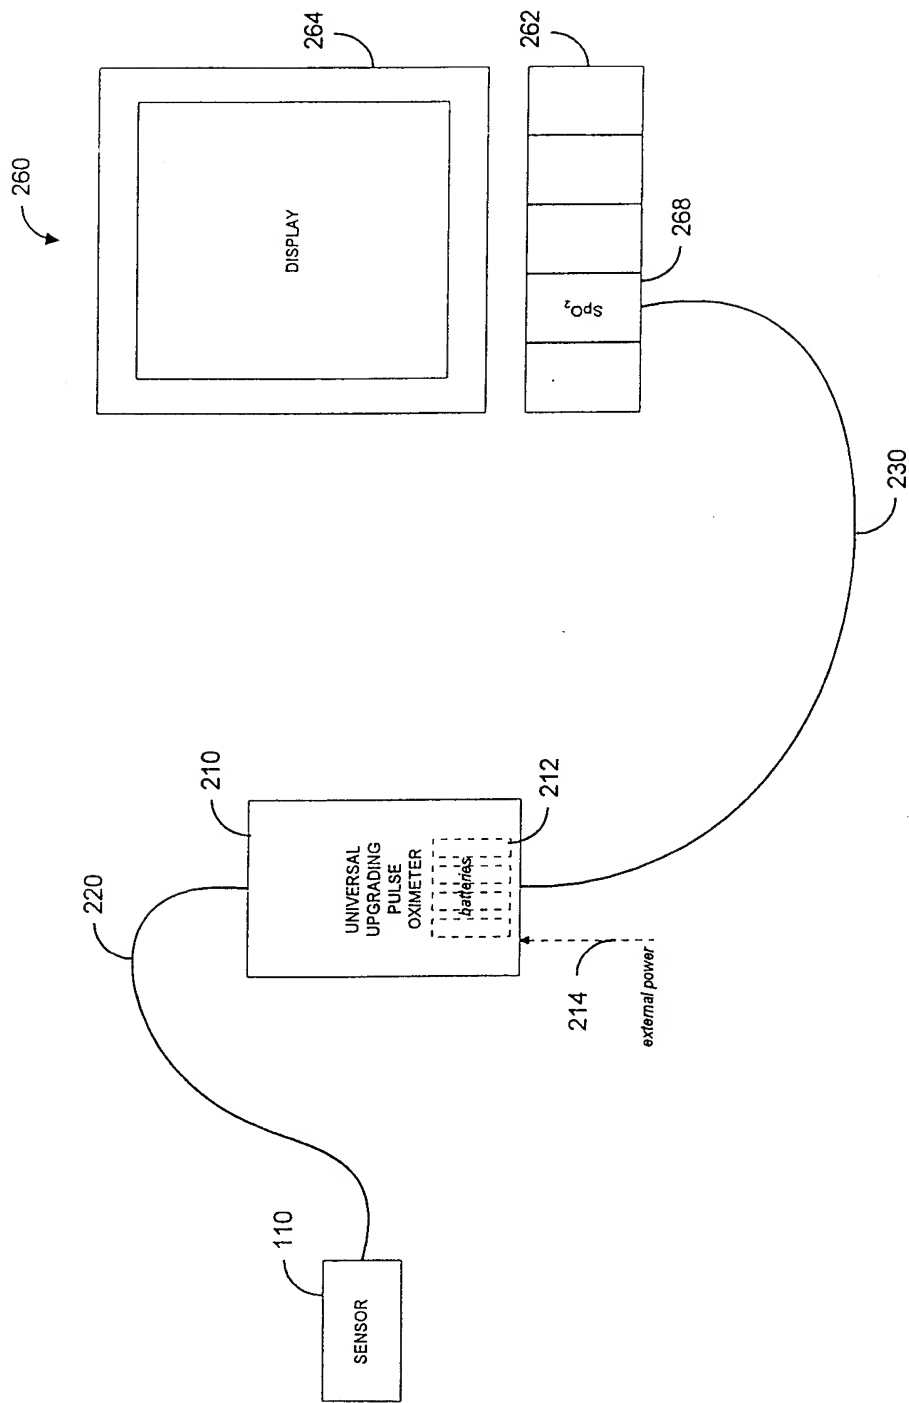


FIG. 2

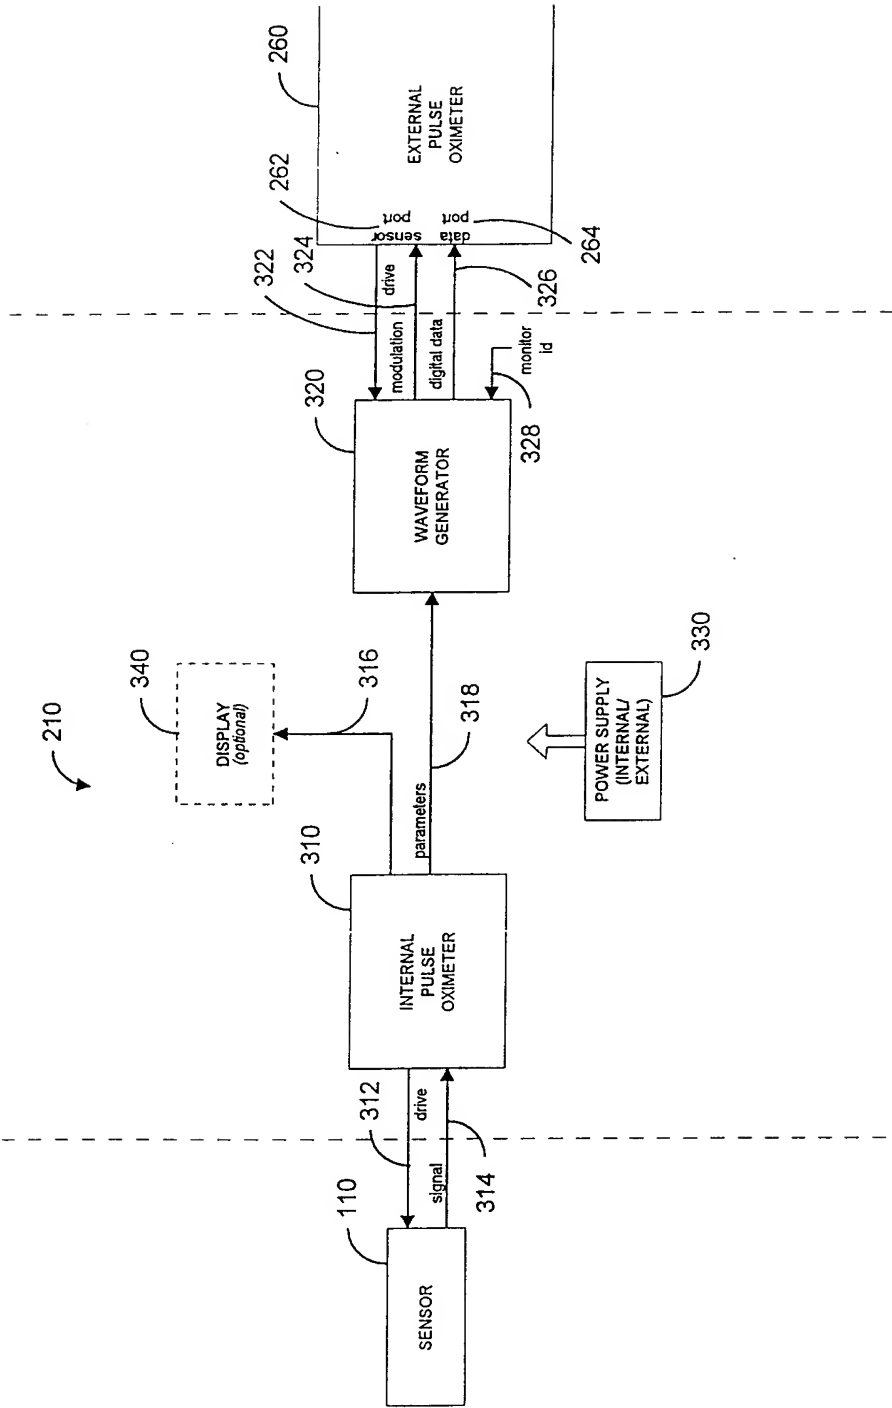


FIG. 3

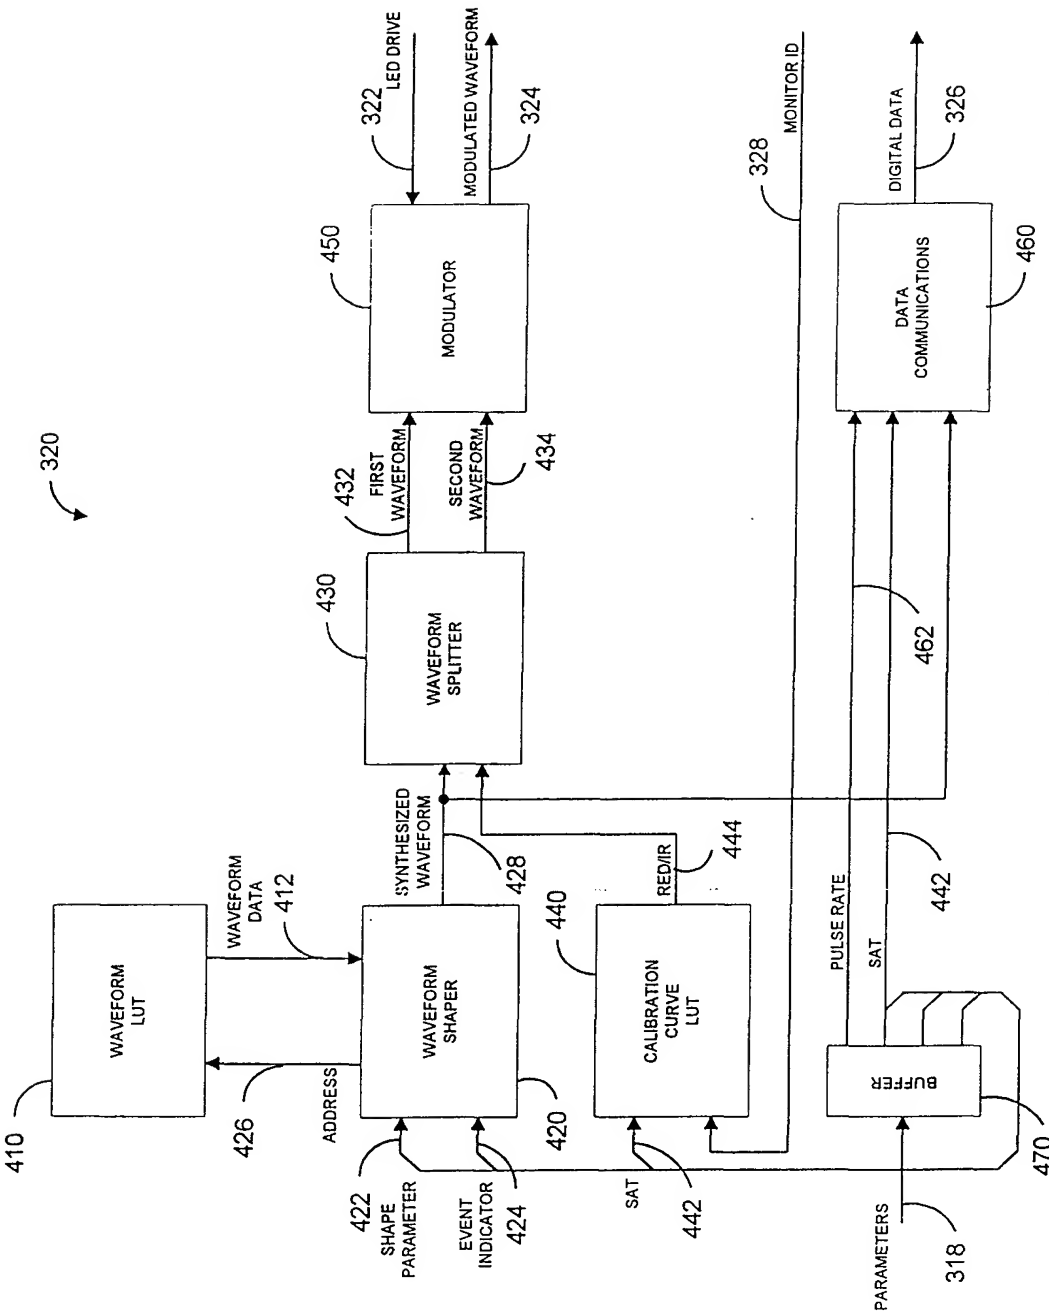


FIG. 4

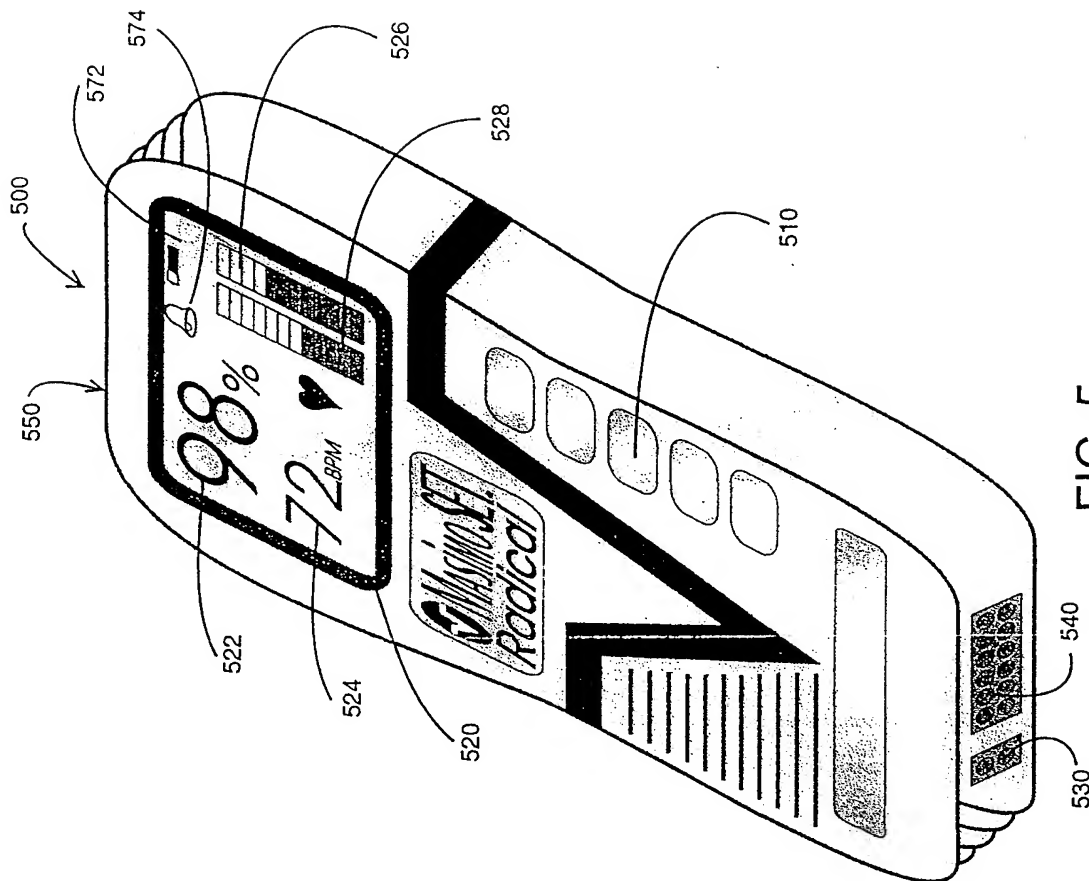


FIG. 5

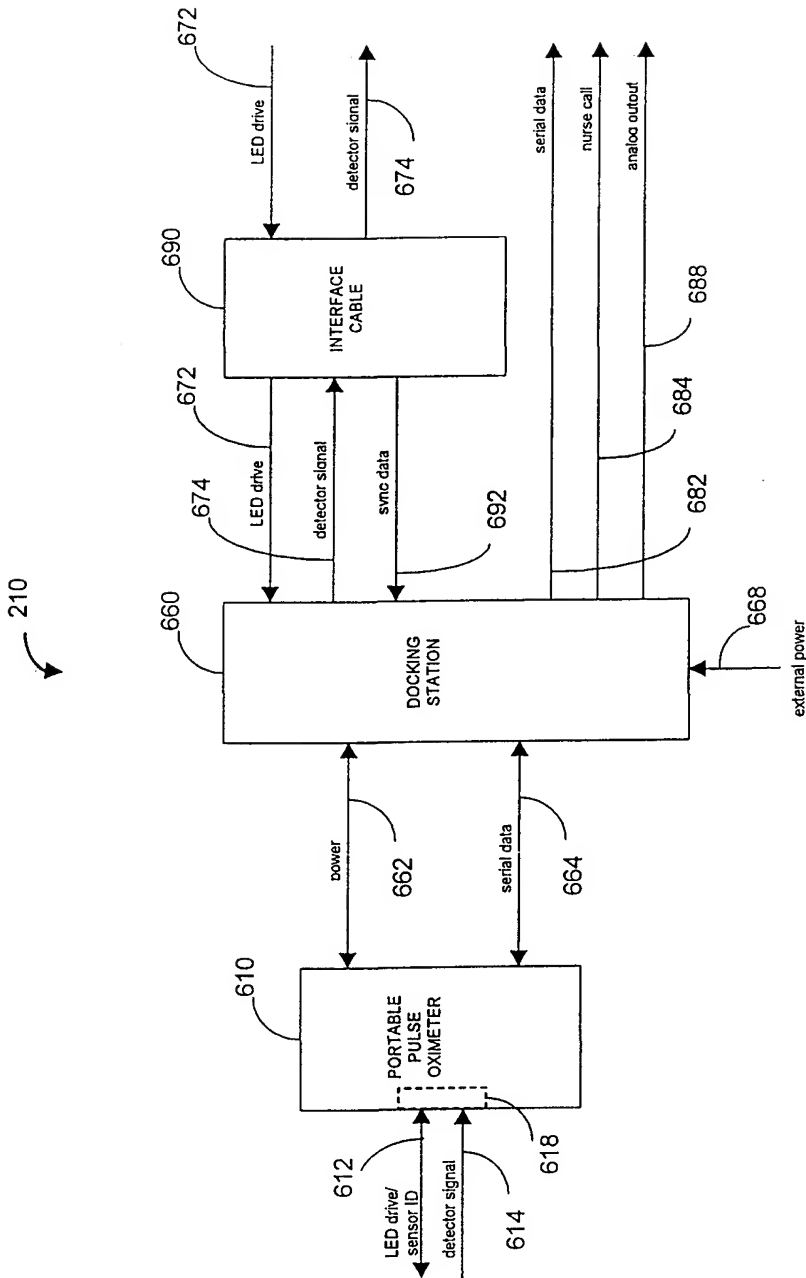


FIG. 6

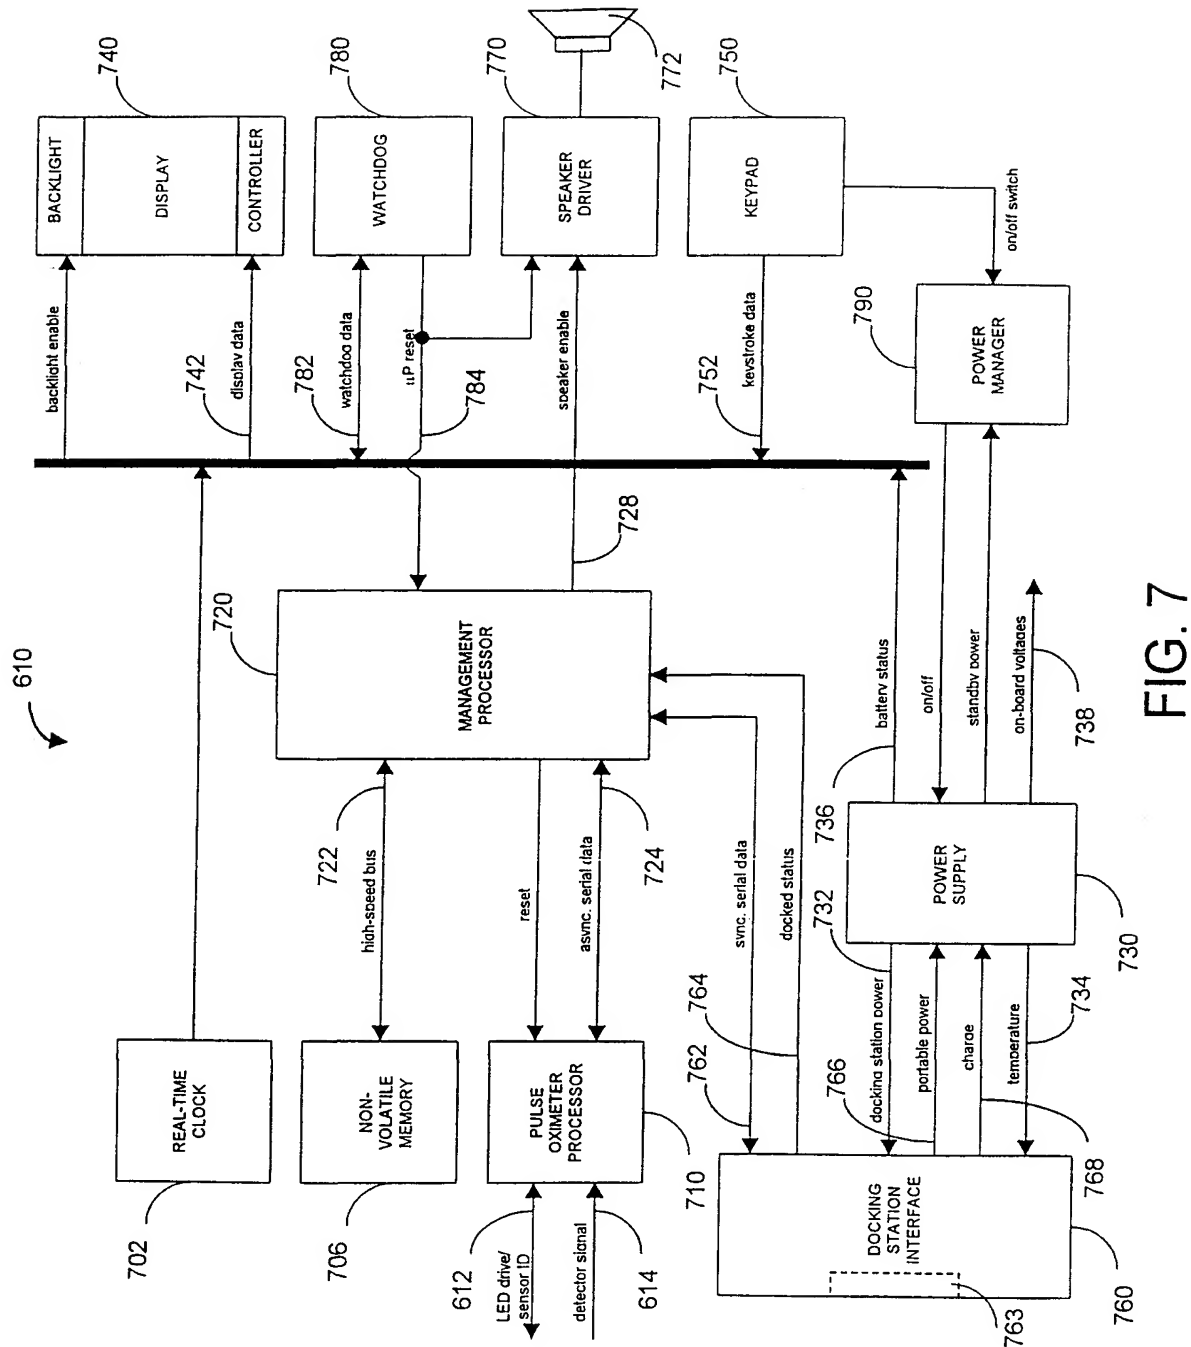


FIG. 7



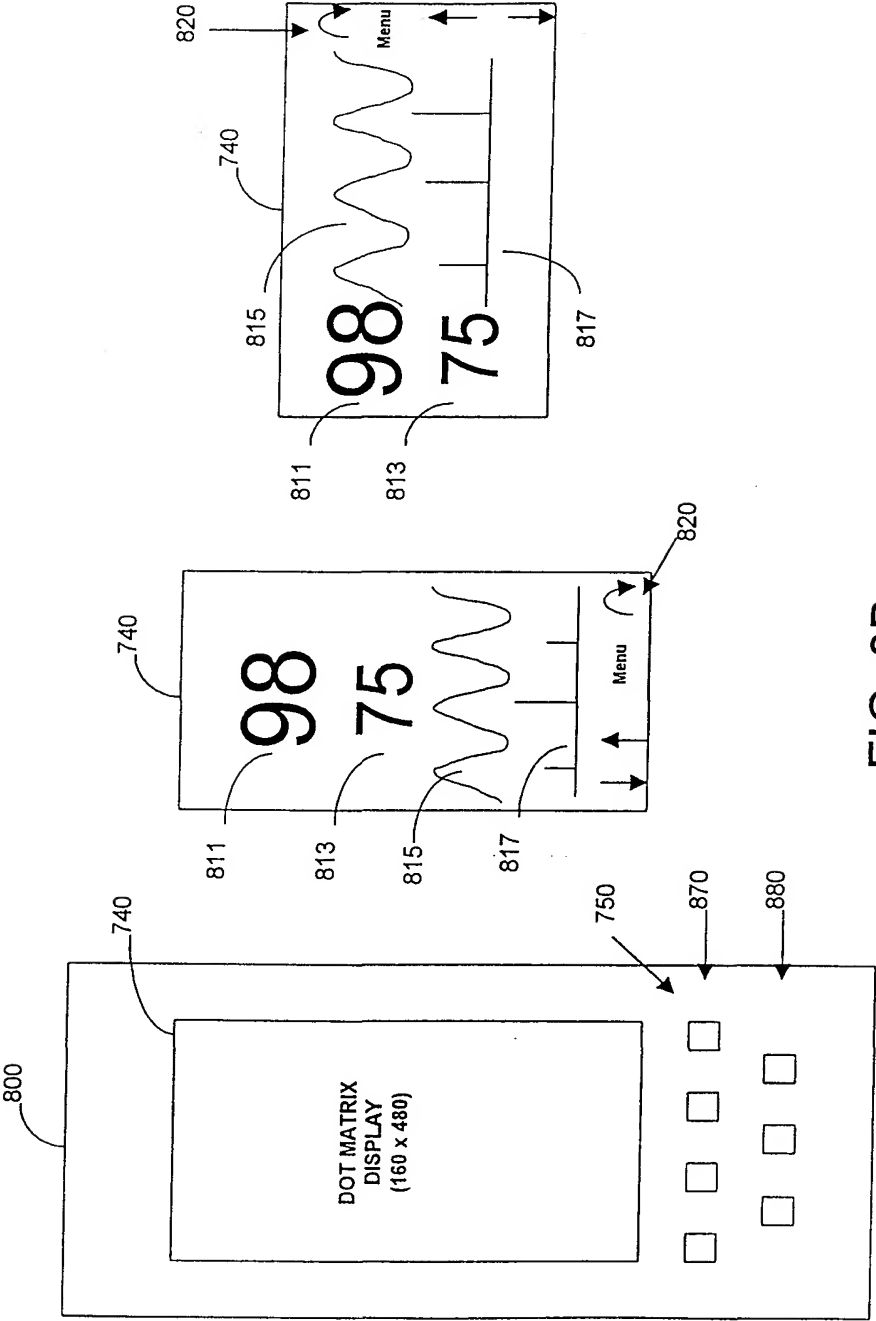


FIG. 8A

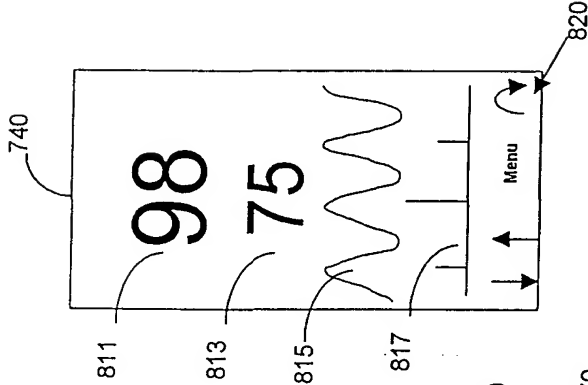


FIG. 8B

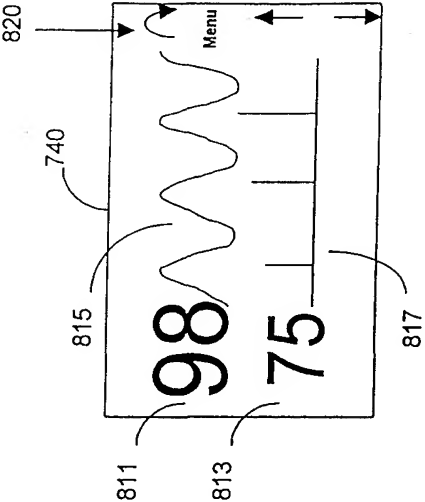


FIG. 8C

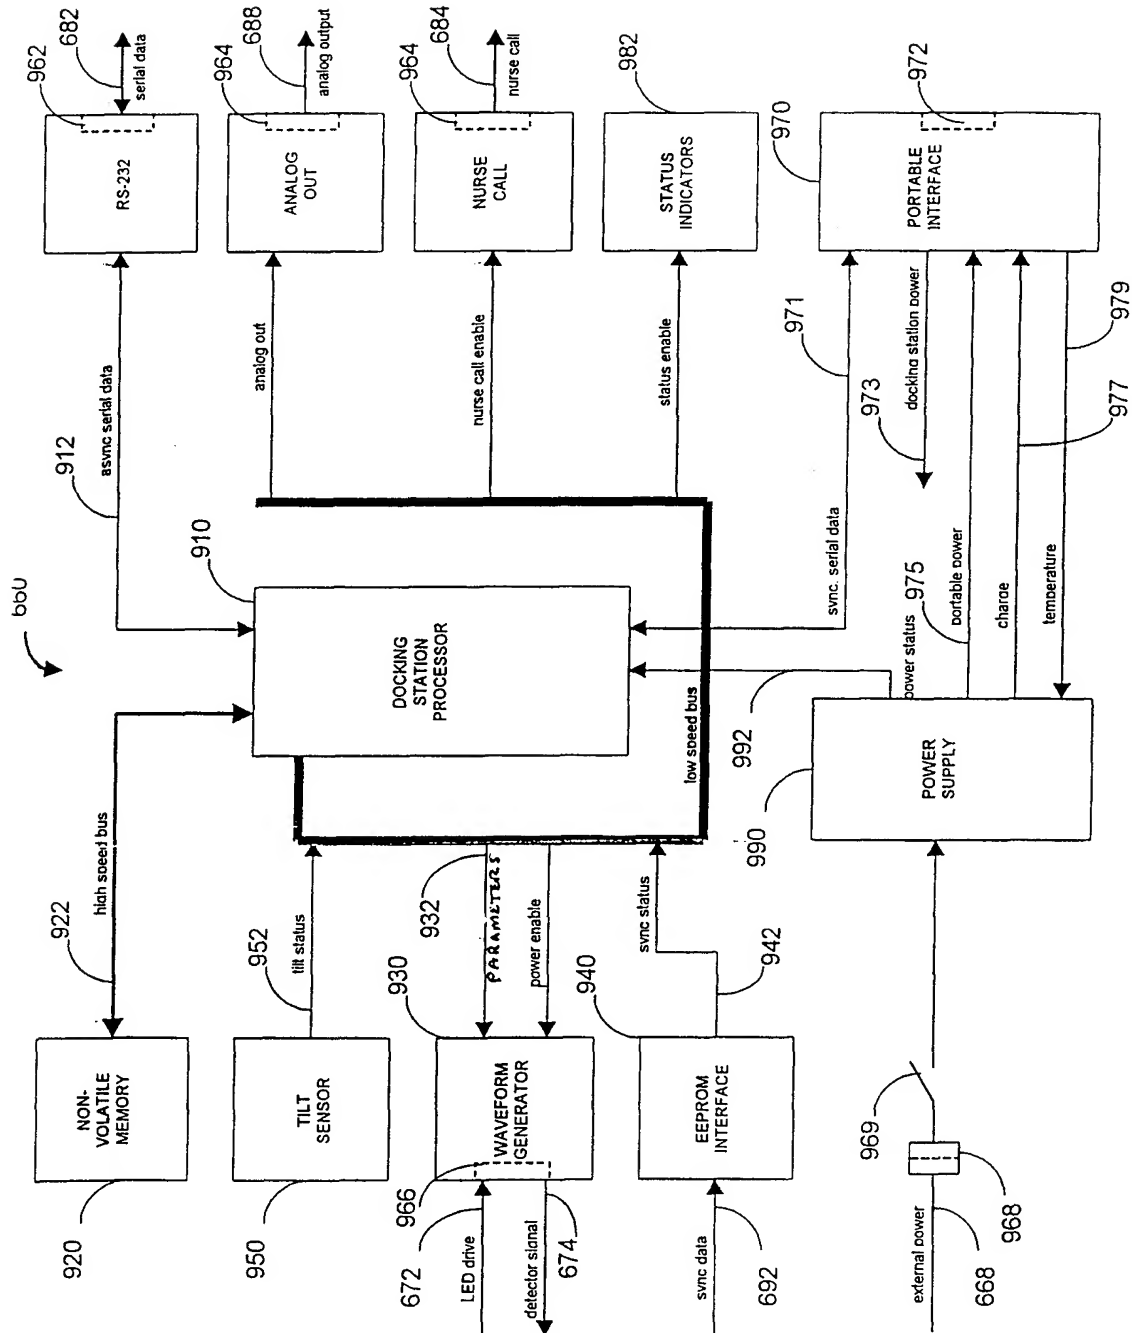


FIG. 9

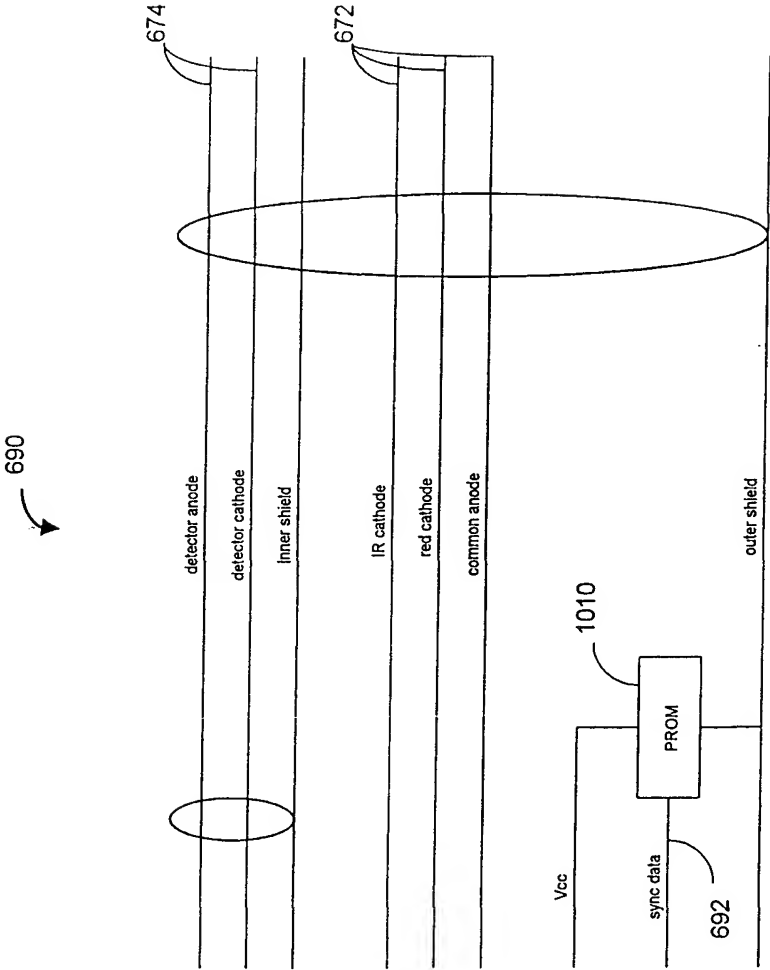


FIG. 10

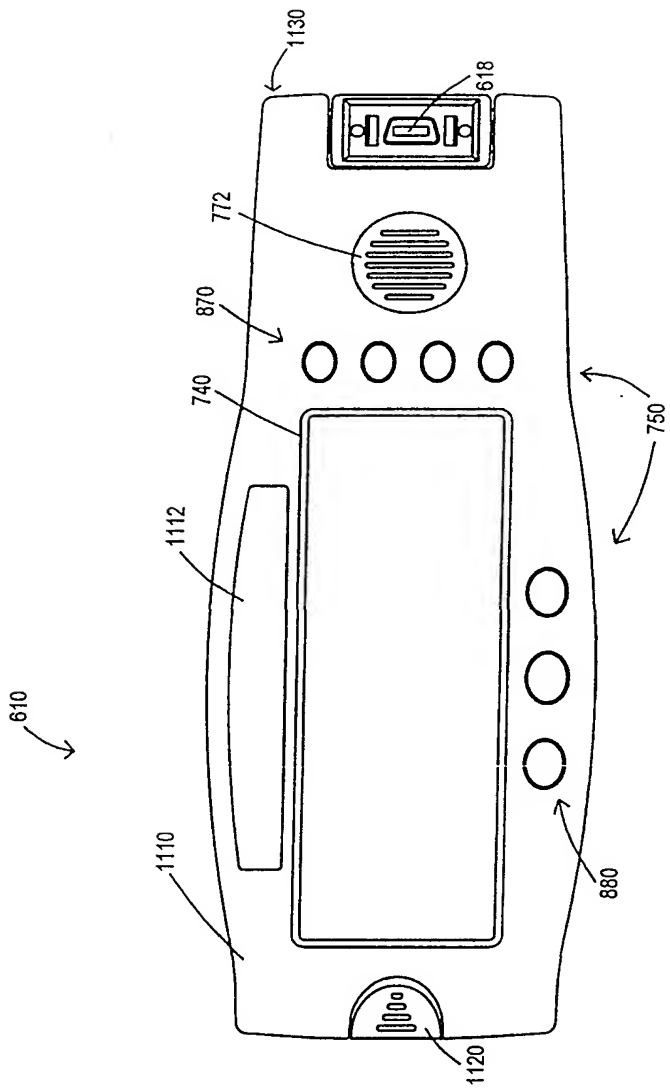


FIG. 11A

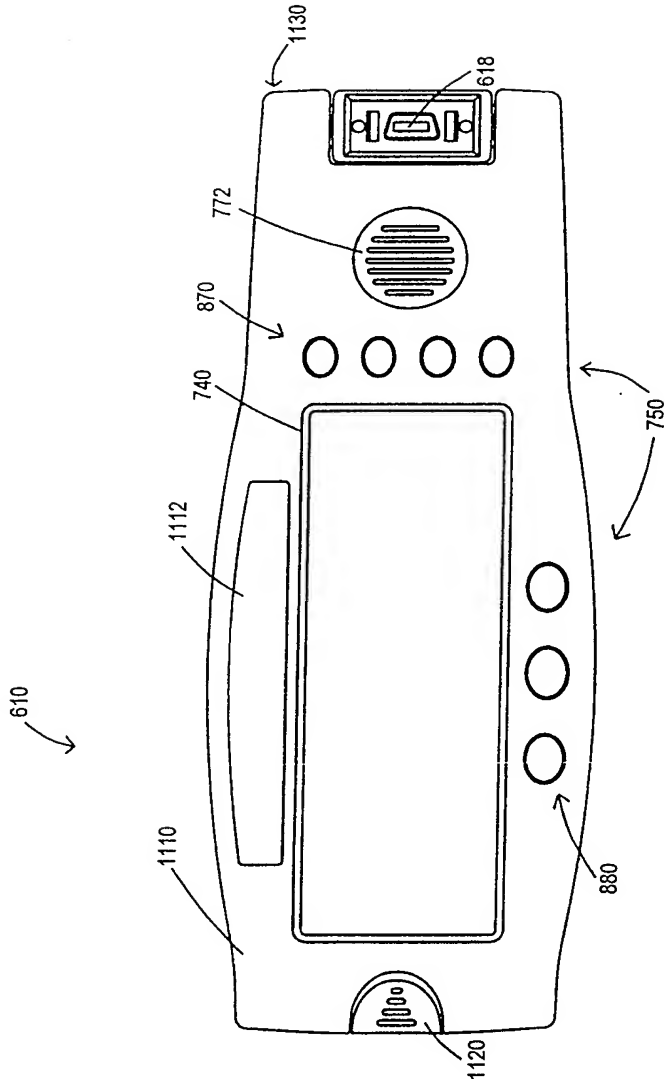


FIG. 11B

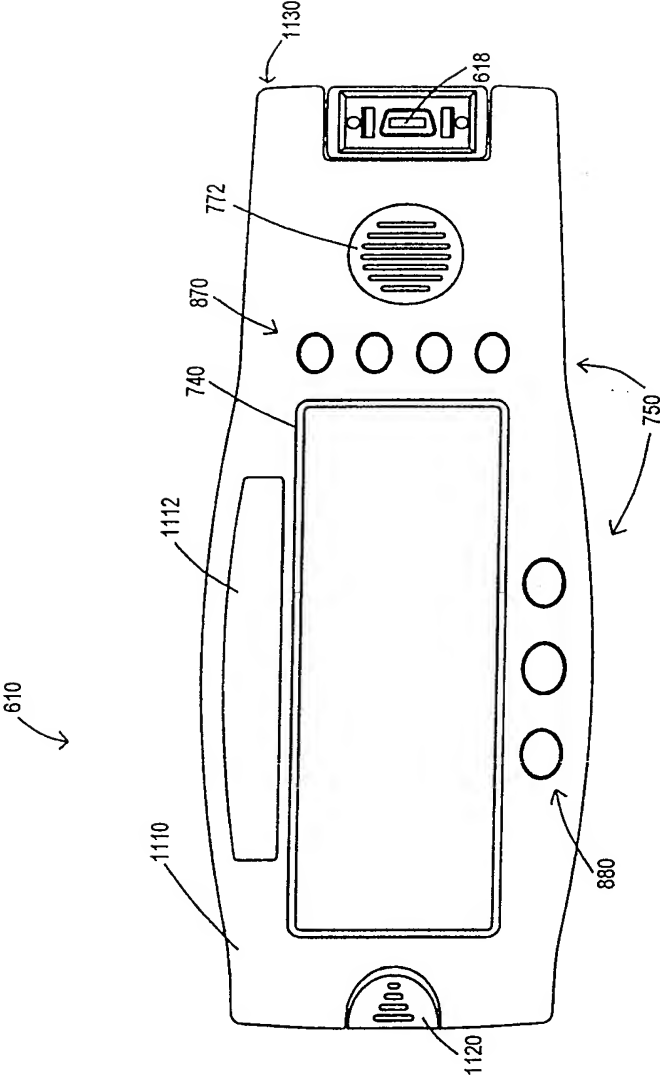


FIG. 12A

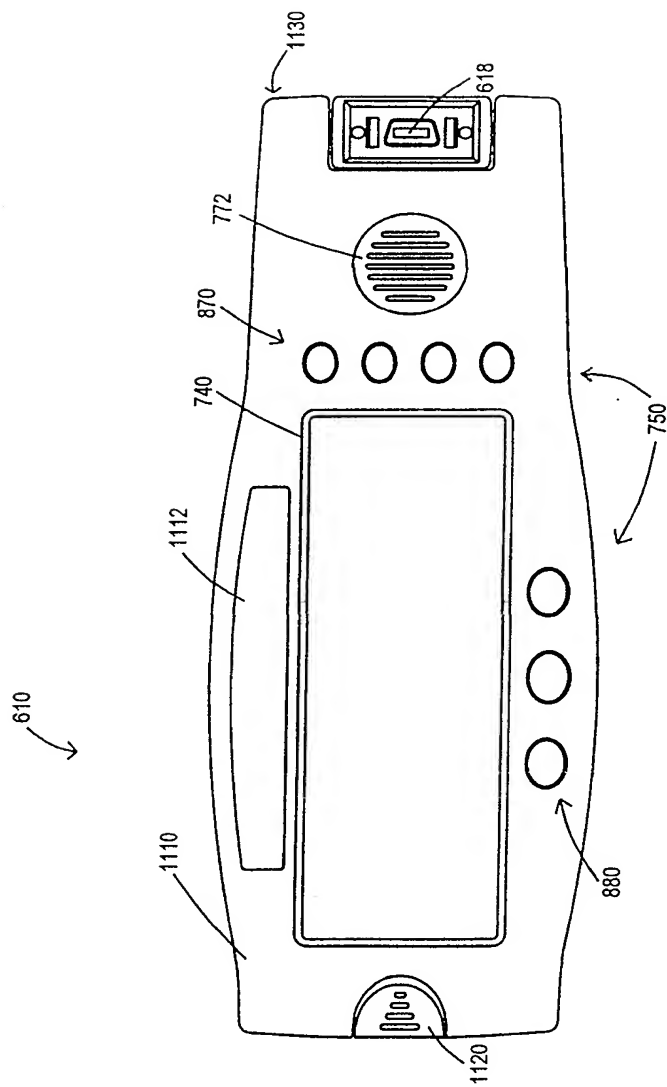


FIG. 12B

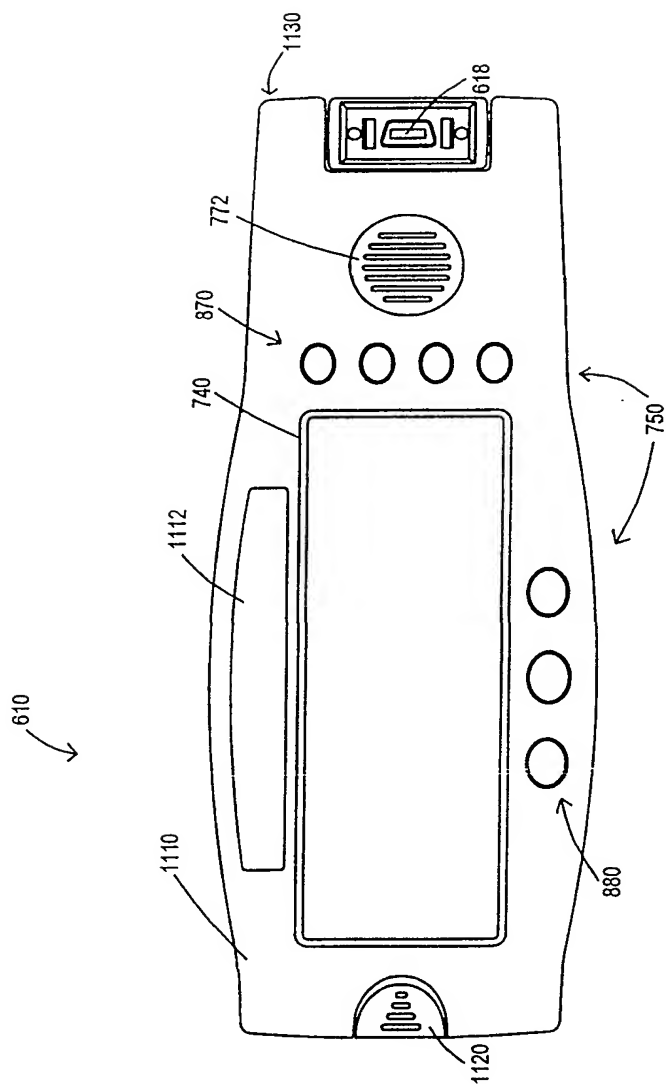


FIG. 13



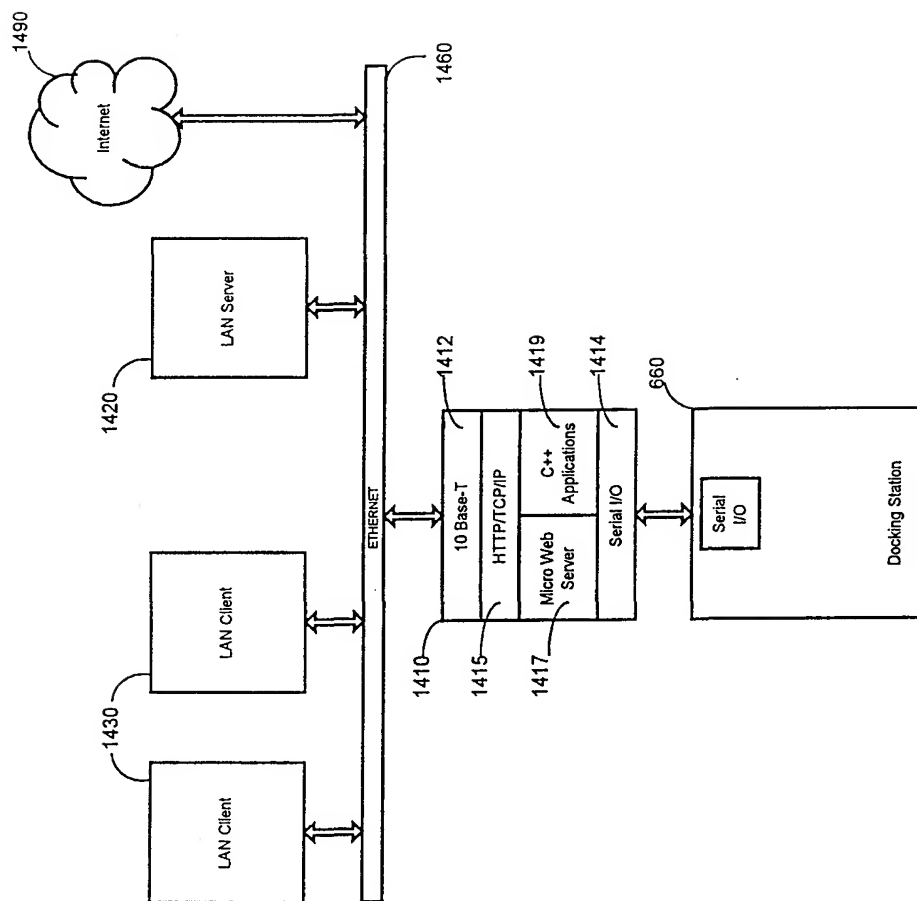


FIG. 14

# INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 00/01884

## A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61B5/00

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 97 22293 A (NELLCOR PURITAN BENNETT INC.) 26 June 1997 (1997-06-26)	1,6,12, 15-17
A	page 4, line 27 -page 6, line 34	21-26,31
A	page 9, line 29 -page 10, line 22	32,43-45
	page 13, line 27 - line 37	
	page 16, line 21 -page 17, line 4	
P,A	US 5 931 791 A (W.E. SALTZSTEIN ET AL.) 3 August 1999 (1999-08-03)	1,6,7, 12-16
A	column 2, line 58 -column 3, line 3	31,33,34
	column 3, line 41 - line 65	

☐ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

### \* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

6 June 2000

Date of mailing of the international search report

14/06/2000

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Rieb, K.D.

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 00/01884

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
WO 9722293	A	26-06-1997	US 5807247 A	15-09-1998
			AU 1420797 A	14-07-1997
			CA 2238958 A	26-06-1997
			DE 69604700 D	18-11-1999
			DE 69604700 T	31-05-2000
			EP 0871396 A	21-10-1998
<hr/>				
US 5931791	A	03-08-1999	NONE	
<hr/>				